


White Paper

Summary of new ISO standards: ISO 6789-1:2017 and ISO 6789-2:2017 For Hand Torque Tools.

March 2017

Additional Information – May 2017

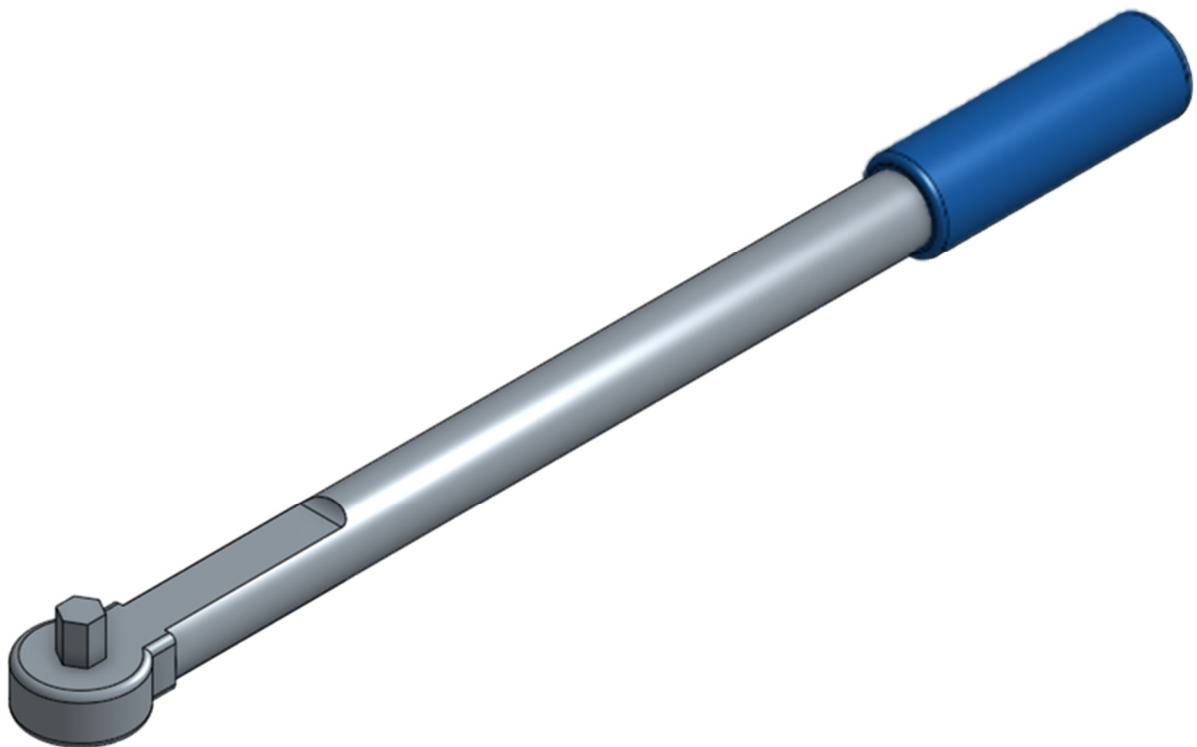

Advanced Witness Systems Ltd.

1. Introduction

This paper gives a brief summary of the main differences between the new standard, ISO 6789:2017 parts 1 & 2, and the standard it has superseded, ISO 6789:2003.

The standard has evolved from 1 single 22 page document to 2 documents totalling 63 pages, with annexes. Whilst this at first appears a huge change, it is hoped this short briefing paper will explain some of the more notable differences.

2. ISO 6789-1:2017 (Part 1)

Part 1 is much like the superseded standard, and concerns the performance and conformity of the torque tool.

On the whole this has not changed, apart from more detailed clarification in certain areas, such as the specified measuring range and the torque tool scales, dials and displays.

The new standard does add a section on the effect of geometric changes of the torque tool, on the torque value, and dependent on the load application point.

The most notable addition is the requirement for a Declaration of Conformance, which must be supplied with the tool. The standard details the required contents of this declaration. These consist of 16 items.

3. ISO 6789-2:2017 (Part 2)

Part 2 concerns the calibration of the torque tool, and requirements of the testing equipment. Additionally is the inclusion of uncertainties of the calibration. This comprises of 7 uncertainties. These being:

w_r – *Uncertainty due to the variation in the scale, dial or display resolution*

w_{rep} – *Uncertainty due to reproducibility of torque tools*

w_{od} – *Uncertainty due to geometric effects of the output drive of the torque tool*

w_{int} – *Uncertainty due to geometric effects of the interface between the output drive of the torque tool and the calibration system*

w_l – *Uncertainty due to the variation of the force loading point*

w_{re} – *Uncertainty due to the repeatability*

w_{md} – *Relative standard measurement uncertainty of the measurement device at the target torque*

It takes into consideration not only the torque tool itself, the variables such as its square drive and possible load application points, but also the adapter on the torque tool and test equipment.

It details how a number of extra operations of the torque tool have to be performed in order to quantify these uncertainties and for compliance with the new standard.

This full calibration process requires that the number of testing operations increases from 35 in the old standard, and to a maximum of 168 in the new.

For example, for each direction of calibration, the number of testing operations (exercises (Ex) and readings (Re)) for each type & class of torque tool will be:

Type & Class	Recorded Measurements for Calibration		Uncertainties						Total Number of Testing Operations	
	Ex	Re	w_{rep}	w_{od}^*		w_{int}^*		w_l^*		
			Re	Ex	Re	Ex	Re	Ex		Re
All Type I. Type II Classes A, D & G	3	15	20	5	40	5	40	5	20	153
Type II Classes B, C, E & F	3	10	40	5	40	5	40	5	20	168

*Note: It is to be hoped that manufacturers can type test 10 of each of their models to provide the variation figures (b_{od}, b_{int}, b_l) as default values, which can be used to generate the uncertainty figures (w_{od}, w_{int}, w_l respectively) to reduce the number of tests performed by the calibration laboratories. If all of these are supplied by the manufacturer, the total number of testing operations is reduced by 115.

It also requires control of the adapters, these ideally being precision adapters, which are permanently identified, recorded, and will assist in reducing the uncertainties of measurement.

Annex C outlines the method and minimum requirements for the calibration of the torque measurement device, and the estimation of its measurement uncertainty. However, the standard allows for existing torque calibration standards, such as the BS7882 standard to be used where the calibration laboratory is operating to the ISO 17025 standard, and as such has traceability.

Additional Information – May 2017:

It is to be noted that Tolerances, as specified, are $\pm 4\%$ or $\pm 6\%$ depending upon range, are applicable to the certificate of conformity only. Conformity to 6789-1 calculates the Relative Measurement Deviation differently than 6789-2 calibration Relative Measurement Error. The result of this is that though a new wrench could be shown to conform to the tolerance requirements, and immediate calibration could show the measurement error to be outside of the $\pm 4\%$ or $\pm 6\%$. This could present difficulties for manufacturers, users and accreditation authorities.

4. Summary

There are large implications for the calibrators and manufacturers of torque tools, maintaining their quality control and accreditation, and thereby conforming to this revised standard. All the above can be quite onerous in its own right and additional calculations require comprehensive spreadsheets.

Advanced Witness Systems Ltd (AWS Ltd) can greatly assist in this with its new Kepler 4 software program to lead and control both the process in calibration, to produce the required results and certificates. AWS Ltd can provide a short course on the detail of the standard when required. Additionally, we can provide precision calibration adapters and calibration instruments to fulfil the need. Please contact us for more information.

Disclaimer: The information in this white paper is believed to be fair and accurate but represents the view of the staff of AWS Ltd. and should not be used for any specific purpose other than that intended, which is to encourage further questions, understanding and debate of the new standard.



Advanced Witness Systems Ltd.

Unit 8 Beaumont Business Centre,
Beaumont Close,
Banbury.
OX16 1TN
Tel: +44 (0) 1295 266939
Email: sales@awstorque.co.uk
www.awstorque.co.uk

Registered in England Company Number: 2565074