NOVANCED WITNESS SYSTEMS LTD

)24


MEASUREMENT ANI ATION CATALOGUE

LIBRATION

¢

ORQUE

2(

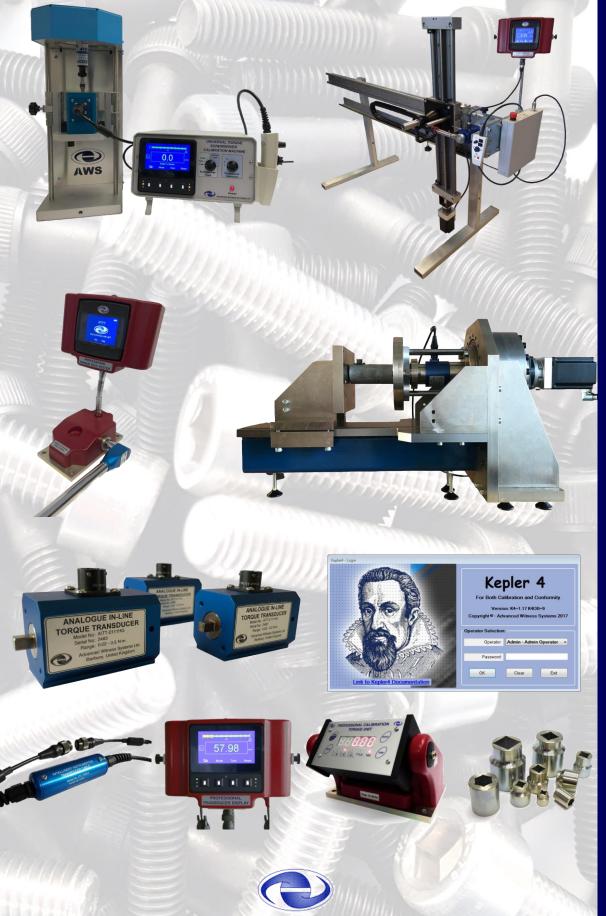

Advanced Witness Systems Ltd.

NDVANCED WITNESS SYSTEMS LTD TORQUE MEASUREMENT & CALIBRATION CATALOGUE 2024

INDEX About Us Testimonials	PAGE 2 3
Torque Transducers I SERIES Transducers A SERIES Transducers N SERIES Transducers	4-27 4-11 12-19 20-27
Transducer Displays & Bench Testers Professional Transducer Display Professional Torque Tool Tester Professional Calibration Torque Unit	28-31 29 30 31
Transducer Ancillaries Precision Torque Adapters Multiway Transducer Switch Box Intelligent Instrument Transducer Cable Transducer Cables	32-37 33-34 35 36 37
Calibration Machines Universal Torque Wrench Calibration Machine What Creates the UTWCM UTWCM Return on Investment Universal Torque Screwdriver Calibration Machine UTSCM Handle Adapters What Creates the UTSCM UTSCM Return on Investment Universal Torque Calibration Machine Unsupported Calibration Beams 2Nm Calibration Machine	38-54 39-40 41 42 43-44 45-46 47 48 49-50 51-53 54
ADMS Software Kepler Software Comparison Kepler 4 Combined Kepler 4 Conformity Kepler 4 Calibration K Factor Verification Module	55-63 56 57-58 59-60 61-62 63
Wireless Telemetry Load Measurement System Overview Wireless Telemetry Load Display Wireless Telemetry Load Link Wireless Telemetry Load Pin Wireless Telemetry Anti 2-Block	64-74 65-67 68 69-70 71-72 73-74

Advanced Witness Systems Ltd Catalogue 2024 Data was correct at time of publication. Catalogue Page 1

ΛBOUT **ΛWS**

Advanced Witness Systems Ltd is a premier designer of torque calibration and control equipment, meeting national and international standards. Trading for over 25 years, our designers have extensive knowledge and experience in design and manufacture of torque instrumentation and control systems. For over 40 years, our Managing Director has been known internationally as specialist in torque and is heavily involved in developing national and international torque standards. He was also concept designer for the NPL National Torque Calibration Machine. Acclaimed to be and since proven to be one of the most accurate in the world.



We have supplied equipment in a variety of sectors including Aerospace, Sub Sea, Transport, Power Generation and Defence.

Over 30 years ago we first developed our Kepler torque tool calibration software. Now, in its latest version, Kepler 4 is our most advanced torque tool calibration software to date.

Some of the AWS Team

AWS products are designed and manufactured in the UK to comprehensive specifications and rigorously tested to fully comply with national and international standards. We have recently released two new machines for calibration of torque wrenches and torque screwdrivers to meet ISO 6789:2017.

Newly released are two machines to revolutionise torque measuring device calibration to BS EN 7882:2017.





Managing Director Mr Ron Sangster at the National Physical Laboratories where he was contracted as the Concept Designer and Consultant for the Master 2kNm Torque Calibration Machine.

UK based in Banbury Oxfordshire, near junction 11 of the M40, we are easily accessible from anywhere in the country. With our proximity to international airports we can be reached from anywhere in the world.

Testimonials



" The help & willingness to advise from the team at Advanced Witness Systems since the installation has proved to us that we certainly made the correct decision. "

ACCREDITED AUSTRALIAN CALIBRATION LABORATORY " We have found the Advanced Witness Systems machines and software to be an excellent asset to our business and would strongly recommend their products to other " calibration facilities.



specifications.





JOINT INTEGRITY TRAINING PROVIDER "Ron Sangster and his team have provided only the best service in terms of supplying calibration machines and technical support for our business. "

To read the full testimonials, visit www.awstorque.co.uk/support/testimonials.html

Advanced Witness Systems Ltd © 2024						
MANUFACTURER INFORMATION	SUPPLIER INFORMATION					
Advanced Witness Systems Ltd						
Unit 8						
Beaumont business Centre						
Beaumont Close						
Banbury						
Ox16 1TN						
Tel: +44 (0)1295 266939						
Email: sales@awstorque.co.uk						

Advensed With a set Overtained Ltd @ 2024

Data was correct at time of publication. Catalogue Page 3

I SERIES TRANSDUCERS

Our I SERIES Torque Transducers are designed to work with our Professional Transducer Display. We produce Inline, Annular and Rotary I SERIES Transducers from 1Nm to 300,000Nm. They are unique with their inbuilt instrumentation PCB to eliminate signal loss.

I SERIES	PAGE
Intelligent In-line Torque Transducers	5-6
1Nm Intelligent In-line Torque Transducers	7-8
Intelligent Annular Torque Transducers	9-10
Intelligent Rotary Torque Transducers	11

Advanced Witness Systems Ltd Catalogue 2024 Data was correct at time of publication. Catalogue Page 4

INTELLIGENT IN-LINE TORQUE TRANSDUCER

DESCRIPTION

The AWS LTD Intelligent In-Line Torque Transducer range (IITT), is designed to accurately measure torque values, in a variety of industries.

With optimised torque ranges, the transducer contains our Intelligent Instrumentation Package, outputting using CAN-BUS protocol to communicate with the AWS LTD Professional Transducer Display (PTD). This digital communication eliminates signal loss when using long lengths of cable, providing flexibility in communicating with other devices and systems. There is an option (using the In-line Transducer Mounting Bracket, purchased separately) to bench mount the transducer in either a vertical or horizontal position.

A simple 2 step calibration. Stores serial & model number, capacity, calibration coefficient, units of calibration, and conversion to other torque units.

SPECIFICATIONS


Model: IITT-	1011	1012	1013	1014	1015	1016	1070	1017					
Ranges:	0.1- 2.5Nm	0.4- 10Nm	2- 50Nm	10- 250Nm	20- 500Nm	40- 1000Nm	60- 1500Nm	0.1- 3kNm					
Square Drive Size:	1⁄4"	1⁄4"	³ ⁄8"	1/2"	3⁄4"	³ /4"	1"	1 1⁄2"					
Accuracy:	Better tha	n 0.1% of read	ing from 10 to	0 100% of rated	output. See	calibration cert	ificate for full re	esults.					
Modes:	Peak: For 1 st Peak: s	 Run: For Dial-type and Electronic Wrenches and Screwdrivers. Peak: For Cam-type Wrenches and Screwdrivers. 1st Peak: For Click-type Wrenches and Screwdrivers, retains reading until manually cancelled or for 3 seconds if auto cancel option is chosen. Communications via can bus. (use with the AWS PTD-1010 power & display unit). 											
Communications:													
Power and Display:	Requires	only a single D	.C power sup	ply (use with A\	WS PTD-101	0, power and d	lisplay is provid	ded).					
Overload	125%												
capability: Maximum mechanical overload:	160% of ra	ange stated.				E.							
Operating Temperature:	-10°C to +	-10°C to +50°C.											
Connector:		Mil C 26482 series. 6 pin. Shell size 10.											
CE:	2014/30/E	U			~	GENTIN	DUCER						
EMC:	BS EN 61	326-1:2013				INTELLI TRATION	In Like						
NATO Stock No: IITT-1011: 6625-22-623-1635 IITT-1012: 6625-22-623-1636 IITT-1013: 6625-22-623-1635 IITT-1014: 6625-22-623-1635 IITT-1015: 6625-22-623-1641													
		-											


Advanced Witness Systems Ltd © 2024 Data was correct at time of publication. Catalogue Page 5

DIMENSIONS

Model	Dir	nensi	on (mi	m)	Face Mounting	Square	Weight
Model	Α	В	С	D	Tapped Hole*	Drive	(Kg)
IITT-1011	100	75	60	36	M5	1⁄4"	1.0
IITT-1012	100	75	60	36	M5	1⁄4"	1.0
IITT-1013	100	75	60	36	M5	³ ⁄8"	1.0
IITT-1014	115	75	60	40	M5	1⁄2"	1.2
IITT-1015	150	90	75	55	M5	³ /4"	2.6
IITT-1016	150	90	75	55	M5	³ /4"	2.7
IITT-1070	150	90	75	55	M5	1"	2.8
IITT-1017	160	106	95	80	N/A	1 ½"	3.8

*The face mounting holes are in a square, centrally located around the square drive.

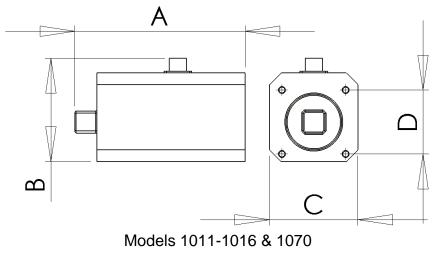

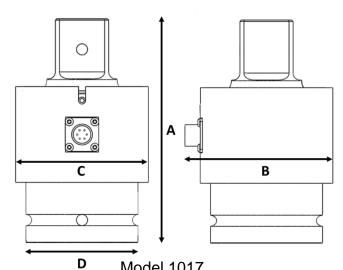

Model 1017

Advanced Witness Systems Ltd © 2024

MANUFACTURER INFORMATION	SUPPLIER INFORMATION
Advanced Witness Systems Ltd	
Unit 8	
Beaumont business Centre	
Beaumont Close	
Banbury	
OX16 1TN	
Tel: +44 (0)1295 266939	
Email: sales@awstorque.co.uk	
Data was correct at ti	me of publication.

Catalogue Page 6

1NM INTELLIGENT IN-LINE TORQUE TRANSDUCER

DESCRIPTION

The AWS LTD Intelligent In-Line Torque Transducer range (IITT), is designed to accurately measure torque values, in a variety of industries.

With optimised torque ranges, the transducer contains our Intelligent Instrumentation Package, outputting using CAN-BUS protocol to communicate with the AWS LTD Professional Transducer Display (PTD). This digital communication eliminates signal loss when using long lengths of cable, providing flexibility in communicating with other devices and systems.

There is an option (using the In-line Transducer Mounting Bracket, purchased separately) to bench mount the transducer in either a vertical or horizontal position.

This transducer incorporates a mechanical overload protection stop at to prevent damage to the transducer. This transducer is either Male SQ drive to Male SQ drive or Male SQ drive to HEX drive. There are 2x M4 threaded holes in the reaction end and bottom surfaces for bolting.

A simple 2 step calibration.

Stores serial & model number, capacity, calibration coefficient, units of calibration, and conversion to other torque units.

SPECIFICATIONS

Canbus

appropriate software.

150% with stop

-10°C to +50°C.

2014/30/EU

Mil C 26482 series.

6 pin. Shell size 10.

BS EN 61326:2007

Model: IITT-	1111	1111H	1018	1018H
Ranges:	0.02-0.5Nm	0.02-0.5Nm	0.04-1Nm	0.04-1Nm
Drive Size:	1⁄4" SQ	1⁄4" HEX	1⁄4" SQ	1⁄4" HEX

Accuracy: Modes: Better than 0.1% of reading from 10 to 100% of rated output. See calibration certificate for full results. **Run:** For Dial-type and Electronic Wrenches and Screwdrivers.

MOUES.

Peak: For Cam-type Wrenches and Screwdrivers.
 1st Peak: For Click-type Wrenches and Screwdrivers, retains reading until manually cancelled or for 3 seconds if auto cancel option is chosen.

AWS Professional Display Model 1010 or External Power Supply 10V and canbus or PC display units with

Communication:

Capacity: Power and Display: Maximum

Overload

mechanical overload: Operating Temperature: Connector:


CE: EMC:




Advanced Witness Systems Ltd © 2024 Data was correct at time of publication. Catalogue Page 7

DIMENSIONS

Model	Dimension (mm)									
	А	В	С	D	Е	F	G	Η		
IITT-1111	82	55	40	25	25	10	12	16	44	
IITT-1018	82	55	40	25	25	10	12	16	44	



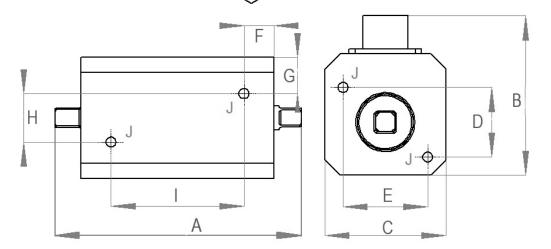

Mounting Tapped Hole "J"	Square Drive	Weight (Kg)
M4	Male ¼"	0.3

Advanced Witness Systems Ltd © 2024							
MANUFACTURER INFORMATION SUPPLIER INFORMATION							
Advanced Witness Systems Ltd							
Unit 8							
Beaumont business Centre							
Beaumont Close							
Banbury							
Ox16 1TN							
Tel: +44 (0)1295 266939							
Email: sales@awstorque.co.uk							

DESCRIPTION

The AWS Intelligent Annular Torque Transducer range (IATT), is designed to accurately measure torque values, in a variety of industries. They function either as a reaction torque transducer taking the reaction torque through the transducer, or with additional drive plates, attached to the flanges, to convert them to direct drive inline transducers.


With optimised torque ranges, the transducer contains our Intelligent Instrumentation Package, outputting using CAN-BUS protocol to communicate with the AWS Professional Transducer Display (PTD). This digital communication eliminates signal loss when using long lengths of cable, providing flexibility in communicating with other devices and systems.

SPECIFICATIONS


Model: IATT-	1038	1039	1031	1032	1033	1034	1035	1046	1036	1037	
Ranges (kNm):	2	3	5	10	20	50	100	120	200	300	
Accuracy: Better than 0.1% of reading from 10 to 100% of rated output. See calibration certificate for full results.											
Modes:	 Run: For Dial-type and Electronic Wrenches and Screwdrivers. Peak: For Cam-type Wrenches and Screwdrivers. 1st Peak: For Click-type Wrenches and Screwdrivers, retains reading until manually cancelled or for 3 seconds if auto cancel option is chosen. 										
Communications:	Communica	Communications via CAN-BUS. (When used with the AWS PTD that converts and displays the signals, showing mode selected, transducer details and output in RS232 serial form).									
Power and Display: Overload capability:	Requires on (when used 125%				ay is provic	led).					
Maximum mechanical overload:	160% of ran	ge stated.			6				1		
Operating Temperature:	-10°C to +50)°C.								2	
Temperature coefficient:	On Zero: 0.0 On Span: 0.						0	0			
Connector:	MIL C 2648 6 pin. Shell				-	10	0			10	
CE:	2014/30/EU					CX.			10		
EMC:	BS EN 6132	26-1:2013									


DIMENSIONS

Dim (mm)	1038/ 1039	1031	1032	1033	1034	1035	1046	1036	1037
Α	39	55	55	70	125	125	125	205	205
В	69	76	76	95	219.92	219.92	219.92	239.92	239.92
С	84.1	177.8	177.8	212	315	315	315	520	520
D	119	184	184	212	315	315	315	520	520
E	99.06	152.4	152.4	195	290	290	290	492	492
F	M5X0.8	M10X1.5	M10X1.5	M10X1.5	M16X2.0	M16X2.0	M16X2.0	M16X2.0	M16X2.0
G	79	77	77	97	126	126	126	130	130
н	84.5	90	90	76	110	110	110	146	146
I	92.5	-	-	-	-	-	-	-	-
J	59	-	-	-	-	-	-	-	-
No. Bolts	24	24	24	24	40	40	40	68	68

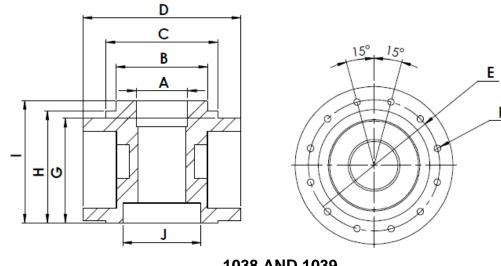


1038 AND 1039





F

1031 AND ABOVE

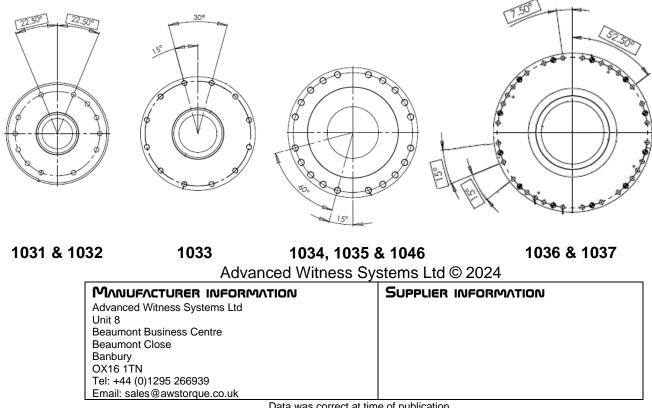

Data was correct at time of publication. Catalogue Page 10

INTELLIGENT ROTARY TORQUE TRANSDUCER

DESCRIPTION

The AWS LTD Intelligent Rotary Torque Transducer range (IRTT), is designed to accurately measure torque values in a rotating shaft, in a variety of industries. With optimised torque ranges, the transducer contains our Intelligent Instrumentation Package, outputting using CAN-BUS protocol to communicate with the AWS LTD Professional Transducer Display (PTD). This digital communication eliminates signal loss when using long lengths of cable, providing flexibility in communicating with other devices and systems. The IRTT can be produced with different adapters depending on its use including square (standard) and keyway (option).

A simple 2 step calibration.

Stores serial & model number, capacity, calibration coefficient, units of calibration, and conversion to other torque units.

SPECIFICATIONS

Tel: +44 (0)1295 266939 Email: sales@awstorque.co.uk

Model: IRTT-	Model: IRTT- 1042		1044	1045	
Ranges: 2-50Nm		10-250Nm	20-500Nm	40-1000Nm	
Square Drive Size:	quare Drive Size: ¾"		³ /4"	3/4"	

Accuracy:	Better than 0.1% of reading from 10 to 100 certificate for full results.	0% of rated output. See calibration			
Modes:		vdrivers. rewdrivers, retains reading until manually cancelled or			
Communications:	for 3 seconds if auto cancel option is chosen. Communications: Communications via can bus. (When used with the AWS PTD-1010 that converts and display signals, shows mode selected, transducer details and output in RS232serial form).				
Power and Display:		used with AWS PTD-1010, power and display is			
	provided).				
Adapter:	The IRTT can be produced with shaft ends	6			
	suitable to its intended function.	A 2 4			
Speed:	Standard 20,000 RPM				
Overload capability:	125%				
Maximum mechanical overload:	160% of range stated.	8			
Operating Temperature range:	-10°C to +50°C.	AWS Life and and a second			
Connector:	Mil C 26482 series. 6 pin. Shell size 10.	Model Model			
CE:	2014/30/EU	Seriel No.			
EMC:	BS EN 61326:2007				
	Advanced Witness Sy	stems Ltd © 2024			
		SUPPLIER INFORMATION			

A Series Transducers

Our A SERIES Torque Transducers are designed to work with any existing analogue torque system.

We produce Inline, Annular and Rotary A SERIES Transducers from 1Nm to 300,000Nm.

A SERIES	PAGE
Analogue In-line Torque Transducers	13-14
1Nm Analogue In-line Torque Transducers	15-16
Analogue Annular Torque Transducers	17-18
Analogue Rotary Torque Transducers	19

Advanced Witness Systems Ltd Catalogue 2024 Data was correct at time of publication. Catalogue Page 12

ANALOGUE IN-LINE TORQUE TRANSDUCER

DESCRIPTION

The AWS LTD Analogue In-Line Torque Transducer range (AITT), is designed to accurately measure torque values, in a variety of industries.

With optimised torque ranges, the transducer uses a standard analogue connection through a male MIL C connector, from a full active Wheatstone bridge, outputting a mV reading. There is an option (using the In-line Transducer Mounting Bracket, purchased separately) to bench mount the transducer in either a vertical or horizontal position.

SPECIFICATIONS

Model: AITT-	2011	2012	2013	2014	2015	2016	2070	2017
Ranges:	0.1- 2.5Nm	0.4- 10Nm	2- 50Nm	10- 250Nm	20- 500Nm	40- 1000Nm	60- 1500Nm	0.1- 3kNm
Square Drive Size:	1⁄4"	1⁄4"	³ ⁄8"	1/2"	³ /4"	³ /4"	1"	1 1⁄2"

Accuracy:	Better than 0.1% of reading from 10 to 100% of rated of	output. See calibration certificate for full results.
Signal output	2 mV/V Strain gauge	
Communication:	mV analogue output	
Bridge Impedance	350 Ω	
MAX Voltage and Current Requirement	10V DC 30mA	
Power and Display:	Requires a stable DC power supply and mV reading meter.	
Overload capability:	125%	
Maximum mechanical overload:	160% of range stated.	• ***•
Operating Temperature:	-10°C to +50°C.	IN-LUCER TRANSDUCER
Connector:	Mil C 26482 series. 6 pin. Shell size 10.	TOR OUE No. 1050 Normal IN Section Section Section
CE: EMC:	2014/30/EU BS EN 61326:2007	






Advanced Witness Systems Ltd © 2024 Data was correct at time of publication. Catalogue Page 13

DIMENSIONS

Model Dimension (mm)			m)	Face Mounting	Square	Weight	
Model	А	В	С	D	Tapped Hole*	Drive	(Kg)
AITT-2011	100	75	60	36	M5	1⁄4"	1.0
AITT-2012	100	75	60	36	M5	1⁄4"	1.0
AITT-2013	100	75	60	36	M5	³ ⁄8"	1.0
AITT-2014	115	75	60	40	M5	1/2"	1.2
AITT-2015	150	90	75	55	M5	3/"	2.6
AITT-2016	150	90	75	55	M5	³ /4"	2.7
AITT-2070	150	90	75	55	M5	1"	2.8
AITT-2017	160	106	95	80	N/A	1 ½"	3.8

*The face mounting holes are in a square, centrally located around the square drive.

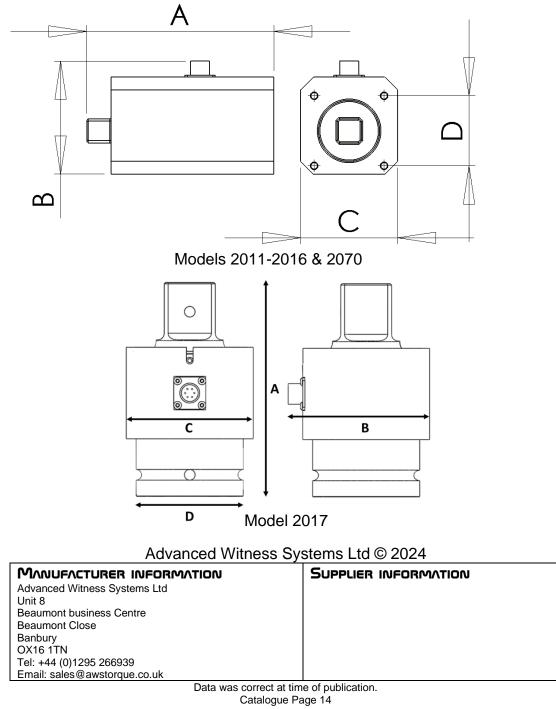

1NM ANALOGUE IN-LINE TORQUE TRANSDUCER

DESCRIPTION

The AWS LTD Analogue In-Line Torque Transducer range (AITT), is designed to accurately measure torque values, in a variety of industries.

With optimized torque ranges, the transducer uses a standard analogue connection through a male MIL C connector, from a full active Wheatstone bridge, outputting a mV/V reading.

There is an option (using the In-line Transducer Mounting Bracket, purchased separately) to bench mount the transducer in either a vertical or horizontal position. The vertical position allows it to be mounted in ISO torque wrench calibration machines.

This transducer incorporates a mechanical overload protection stop to prevent damage to the transducer. This transducer can either be Male SQ drive to Male SQ drive or Male SQ to Male HEX drive. There are 2x M4 threaded holes in the reaction end and bottom surfaces for bolting.


SPECIFICATIONS


Model: AITT-	2111	2111H	2018	2018H	
Ranges:	0.02-0.5Nm	0.02-0.5Nm	0.04-1Nm	0.04-1Nm	
Drive Size:	1/4"	1⁄4" HEX	1⁄4"	1⁄4" HEX	

Accuracy:	Better than 0.1% of reading from 10 to 100% of rated output. See calibration certificate for full results.
Signal output	2 mV/V Strain gauge
Communication:	mV
Overload Capacity:	120%
Bridge Impedance	350 Ω
MAX voltage and current	10V DC 30mA
requirement Power and Display:	Dedicated mV/V display and power supply.
Maximum	6
mechanical overload:	150% with stop
Operating Temperature:	-10°C to +50°C. Mil C 26482 series
Connector:	Mil C 26482 series. 6 pin. Shell size 10.
CE: EMC:	2014/30/EU BS EN 61326:2007

DIMENSIONS

Madal				Dir	nensio	n			
Model	А	В	С	D	Е	F	G	Н	
AITT-2111	82	53	40	25	25	10	12	16	44
AITT-2018	82	53	40	25	25	10	12	16	44



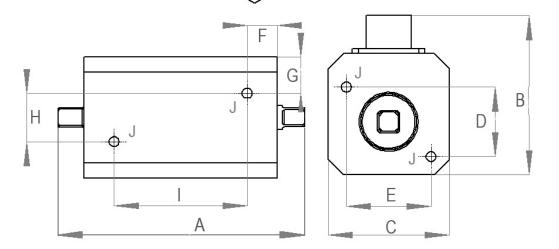

Mounting Tapped Hole "J"	Square Drive	Weight (Kg)
M4	Male ¼"	0.3

Advanced Witness Systems Ltd © 2024							
MANUFACTURER INFORMATION SUPPLIER INFORMATION							
Advanced Witness Systems Ltd							
Unit 8							
Beaumont business Centre							
Beaumont Close							
Banbury							
OX16 1TN							
Tel: +44 (0)1295 266939							
Email: sales@awstorgue.co.uk							

ANALOGUE ANNULAR TORQUE TRANSDUCER

DESCRIPTION

The AWS Analogue Annular Torque Transducer range (AATT), is designed to accurately measure torque values, in a variety of industries. They function either as a reaction torque transducer taking the reaction torque through the transducer, or with additional drive plates, attached to the flanges, convert them to direct drive inline transducers.

With optimised torque ranges, the transducer uses a standard analogue connection through a male MIL C connector, from a full active Wheatstone bridge, outputting a mV reading.


Specifications

Model: AATT-	2029	2030	2031	2032	2033	2034	2035	2046	2036	2037
Ranges (kNm):	2	3	5	10	20	50	100	120	200	300

Accuracy:	Better than 0.1% of reading from 10 to 100% of rated output. See calibration certificate for full results.
Signal Output	2mv/v
	Strain gauged bridge
Power and Display:	Requires a stable DC power supply and mV reading meter.
Overload capability:	125%
Bridge Impedance	350Ω
Max Voltage and Current Requirement	10V 30mA DC
Maximum mechanical overload:	160% of range stated.
Operating Temperature:	-10°C to +50°C.
Temperature coefficient:	On Zero: 0.01% per °C On Span: 0.03% per °C
Connector:	Mil C 26482 series. 6 pin. Shell size 10.
CE:	2014/30/EU
EMC:	BS EN 61326:2013

DIMENSIONS

	1							1	
Dim (mm)	2029/ 2030	2031	2032	2033	2034	2035	2046	2036	2037
Α	39	55	55	70	125	125	125	205	205
В	69	76	76	95	219.92	219.92	219.92	239.92	239.92
С	84.1	177.8	177.8	212	315	315	315	520	520
D	119	184	184	212	315	315	315	520	520
E	99.06	152.4	152.4	195	290	290	290	492	492
F	M5X0.8	M10X1.5	M10X1.5	M10X1.5	M16X2.0	M16X2.0	M16X2.0	M16X2.0	M16X2.0
G	79	77	77	97	126	126	126	130	130
Н	84.5	90	90	76	110	110	110	146	146
I	92.5	-	-	-	-	-	-	-	-
J	59	-	-	-	-	-	-	-	-
No. Bolts	24	24	24	24	40	40	40	68	68

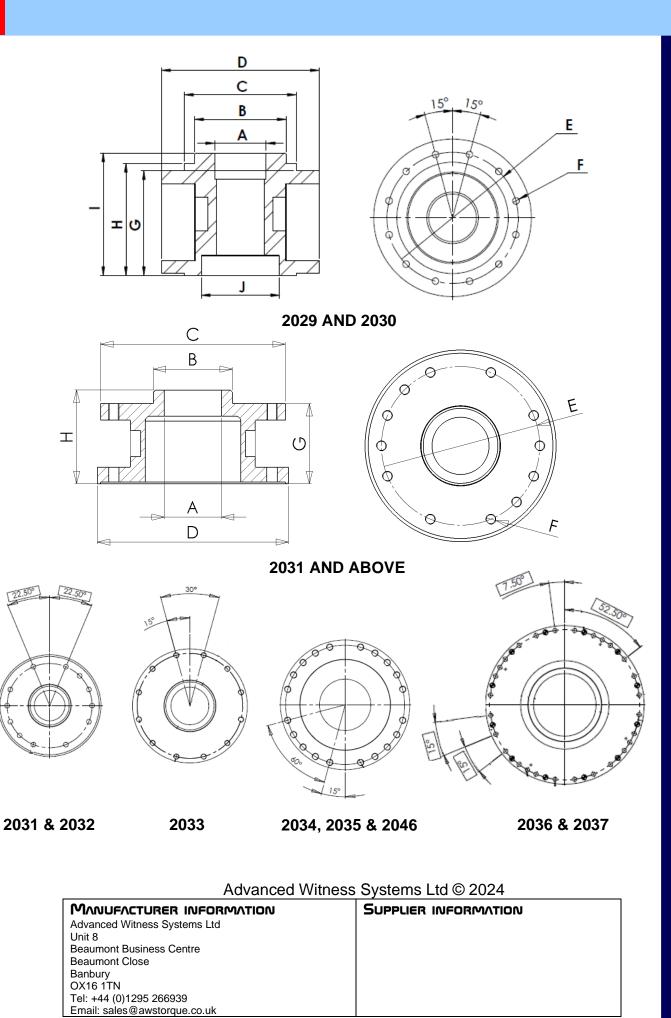

Data was correct at time of publication. Catalogue Page 18

ANALOGUE ROTARY TORQUE TRANSDUCER

DESCRIPTION

The AWS LTD Analogue Rotary Torque Transducer range (ARTT), is designed to accurately measure torque values in a rotating shaft, in a variety of industries.


With optimised torque ranges, the transducer uses a standard analogue connection through a male MIL C connector, from a full active Wheatstone bridge, outputting a mV reading. The ARTT can be produced with different adapters depending on its use including square (standard) and keyway (option).

SPECIFICATIONS

Model: ARTT-	2041	2042	2043	2044	2045
Ranges:	0.4-10Nm	2-50Nm	10-250Nm	20-500Nm	40-1000Nm
Square Drive Size:	1/4"	3/ " /8	1/2"	3/4"	3⁄4"

Δ	~~	urs	acy	
	υu	uic	зсу	•

Accuracy:	Better than 0.1% of reading from 10 to 100% of rated output. See calibration certificate for full results.
Signal Output:	Analogue mV
Communications: Power and Display:	N/A Requires a stable DC power supply and mV reading meter.
Adapter:	The ARTT can be produced with shaft
	ends suitable to its indented function.
Speed:	Standard 20,000 RPM
Overload capability:	125%
Bridge Impedance:	350 Ω
Max Voltage and Current Requirement:	10V DC 30mA
Maximum mechanical overload:	160% of range stated.
Operating Temperature:	-10°C to +50°C.
Connector:	Mil C 26482 series.
	6 pin. Shell size 10.
CE:	2014/30/EU
EMC:	BS EN 61326:2007



Advanced Witness Systems Ltd © 2024

,	
MANUFACTURER INFORMATION	SUPPLIER INFORMATION
Advanced Witness Systems Ltd	
Unit 8	
Beaumont business Centre	
Beaumont Close	
Banbury	
OX16 1TN	
Tel: +44 (0)1295 266939	
Email: sales@awstorque.co.uk	

N SERIES TRANSDUCERS

Our N SERIES Torque Transducers are designed to work with other manufacturer's intelligent display systems.

We produce Inline, Annular and Rotary N SERIES Transducers from 1Nm to 300,000Nm.

N SERIES	PAGE
N-Type In-line Torque Transducers	21-22
1Nm N-Type In-line Torque Transducers	23-24
N-Type Annular Torque Transducers	25-26
N-Type Rotary Torque Transducers	27

Advanced Witness Systems Ltd Catalogue 2024 Data was correct at time of publication. Catalogue Page 20

N-TYPE IN-LINE TORQUE TRANSDUCER

DESCRIPTION

The AWS LTD N-type In-Line Torque Transducer range (NITT), is designed to accurately measure torque values, in a variety of industries.

With optimised torque ranges, the transducer outputs a mV signal proportional to the supply voltage and torque. The transducer contains a memory chip in which a small selection of parameters, including serial number, model number, and calibration value, are held, compatible for setting some manufacturers display units.

There is an option (using the In-line Transducer Mounting Bracket, purchased separately) to bench mount the transducer in either a vertical or horizontal position.

SPECIFICATIONS

Model: NITT-	3011	3012	3013	3014	3015	3016	3070	3017
Ranges:	0.1- 2.5Nm	0.4- 10Nm	2-50Nm	10- 250Nm	20- 500Nm	40- 1000Nm	60- 1500Nm	0.1- 3kNm
Square Drive Size:	1⁄4"	1⁄4"	3⁄8"	1⁄2"	³ /4"	3⁄4"	1"	1 1⁄2"

Accuracy: Better than 0.1% of reading from 10 to 100% of rated output. See calibration certificate for full results. Signal Output: 2mV/V **Communications:** Not Applicable Bridge 350Ω Impedance: 10V DC 30mA Max Voltage and Current **Requirements:** Requires DC power supply and Dedicated mV meter Power and Display: Overload 125% capability: Maximum 160% of range stated. mechanical overload: Operating -10°C to +50°C. Temperature: Mil C 26482 series. Connector: 6 pin. Shell size 10. CE: 2014/30/EU EMC: BS EN 61326:2007






Advanced Witness Systems Ltd © 2024 Data was correct at time of publication. Catalogue Page 21

DIMENSIONS

Model	Di	Dimension (mm)		Face Mounting	Square	Weight	
woder	А	В	С	D	Tapped Hole*	Drive	(Kg)
NITT-3011	100	75	60	36	M5	1⁄4"	1.0
NITT-3012	100	75	60	36	M5	1/4"	1.0
NITT-3013	100	75	60	36	M5	³ ⁄8"	1.0
NITT-3014	115	75	60	40	M5	1/2"	1.2
NITT-3015	150	90	75	55	M6	3/4"	2.6
NITT-3016	150	90	75	55	M6	3/4"	2.7
NITT-3070	150	90	75	55	M6	1"	2.8
NITT-3017	160	106	95	80	N/A	1 1⁄2"	3.8

*The face mounting holes are in a square, centrally located around the square drive.

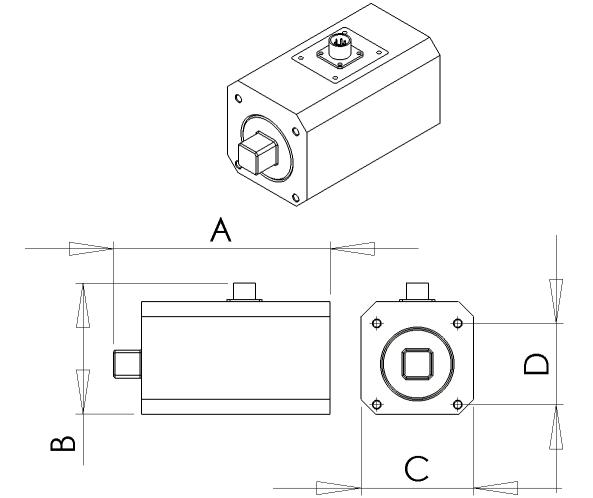

Advanced Witness Systems Ltd © 2024

MANUFACTURER INFORMATION	SUPPLIER INFORMATION
Advanced Witness Systems Ltd	
Unit 8	
Beaumont business Centre	
Beaumont Close	
Banbury	
OX16 1TN	
Tel: +44 (0)1295 266939	
Email: sales@awstorque.co.uk	

1NM N-TYPE IN-LINE TORQUE TRANSDUCER

DESCRIPTION

The AWS LTD N-Type In-Line Torque Transducer range (NITT), is designed to accurately measure torque values, in a variety of industries.

With optimized torque ranges, the transducer uses a standard analogue connection through a male MIL C connector, from a full active Wheatstone bridge, outputting a mV/V reading.

The transducer contains a memory chip in which a small selection of parameters, including serial number, model number, and calibration value, are held, compatible for setting some manufacturers display units.

There is an option (using the In-line Transducer Mounting Bracket, purchased separately) to bench mount the transducer in either a vertical or horizontal position. The vertical position allows it to be mounted in ISO torque wrench calibration machines.

This transducer incorporates a mechanical overload protection stop at 110% of full scale to prevent damage to the transducer. This transducer is can either be Male SQ drive to Male SQ drive or Male SQ to Male HEX drive. There are 2x M4 threaded holes in the reaction end and bottom surface for bolting.

SPECIFICATIONS


Model: NITT-	3111	3111H	3018	3018H
Ranges:	0.02-0.5Nm	0.02-0.5Nm	0.04-1Nm	0.04-1Nm
Drive Size:	1/4"	1⁄4" HEX	1/4"	1⁄4" HEX


Accuracy:	Better than 0.1% of reading from 10 to 100% of rated output. See calibration certificate for full results.
Signal output	2 mV/V Strain gauge
Communication:	Not Applicable
Overload Capacity:	120%
Bridge Impedance	350 Ω
MAX voltage requirement	10V DC 30mA
Power and Display:	Requires DC power supply and Dedicated mV meter
Maximum mechanical overload: Operating Temperature: Connector:	150% with stop -10°C to +50°C. Mil C 26482 series. 6 pin. Shell size 10.
CE: EMC:	2014/30/EU BS EN 61326:2007 IN-EIN- BS EN 61326:2007

Advanced Witness Systems Ltd © 2024 Data was correct at time of publication. Catalogue Page 23

DIMENSIONS

Model		Dimension (mm)							
Model	Α	В	С	D	E	F	G	Н	
NITT-3111	82	53	40	25	25	10	12	16	44
NITT-3018	82	53	40	25	25	10	12	16	44



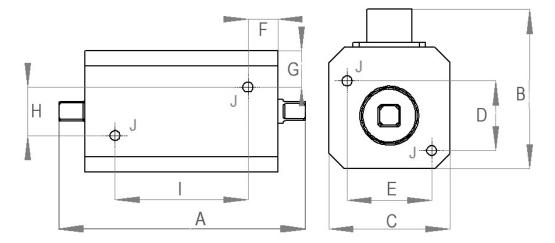

Mounting Tapped Hole "J"	Square Drive	Weight (Kg)
M4	Male ¼"	0.3

Advanced Witness Systems Ltd © 2024

MANUFACTURER INFORMATION	SUPPLIER INFORMATION
Advanced Witness Systems Ltd	
Unit 8	
Beaumont business Centre	
Beaumont Close	
Banbury	
OX16 1TN	
Tel: +44 (0)1295 266939	
Email: sales@awstorque.co.uk	

N-TYPE ANNULAR TRANSDUCER

DESCRIPTION

The AWS N-type Annular Torque Transducer range (NATT), is designed to accurately measure torque values, in a variety of industries. They function either as a reaction torque transducer taking the reaction torque through the transducer, or with additional drive plates, attached to the flanges, convert them to direct drive inline transducers.

With optimised torque ranges, the transducer outputs a mV signal proportional to the supply voltage and torque. The transducer contains a memory chip in which a small selection of parameters, including serial number, model number, and calibration value, are held, compatible for setting some manufacturers display units.


SPECIFICATIONS


Model: NATT-	3038	3030	3031	3032	3033	3034	3035	3046	3036	3037
Ranges (kNm):	2	3	5	10	20	50	100	120	200	300

Accuracy:	Better than 0.1% of reading from 10 to 100% of rated output. See calibration certificate for full results.
Communications:	2 wire EEPROM instrument set up program.
Power and Display:	Can be used with a mV/V display, but is also compatible with other manufacturers' displays.
Overload capability:	125%
Maximum mechanical overload:	160% of range stated.
Maximum bridge supply voltage:	10V
Temperature range:	-10°C to +50°C.
Temperature coefficient:	On Zero: 0.01% per °C On Span: 0.03% per °C
Connector:	Mil C 26482 series. 6 pin. Shell size 10.
CE:	2004/108/EEC
EMC:	BS EN 61326:2013
Signal Output	2mv/v
	Strain gauged bridge
Bridge Impedance	350Ω
Max Power Requirement	10V 20mA DC


DIMENSIONS


Dim (mm)	3038/ 3030	3031	3032	3033	3034	3035	3046	3036	3037
Α	39	55	55	70	125	125	125	205	205
В	69	76	76	95	219.92	219.92	219.92	239.92	239.92
С	84.1	177.8	177.8	212	315	315	315	520	520
D	119	184	184	212	315	315	315	520	520
Е	99.06	152.4	152.4	195	290	290	290	492	492
F	M5X0.8	M10X1.5	M10X1.5	M10X1.5	M16X2.0	M16X2.0	M16X2.0	M16X2.0	M16X2.0
G	79	77	77	97	126	126	126	130	130
Н	84.5	90	90	76	110	110	110	146	146
I	92.5	-	-	-	-	-	-	-	-
J	59	-	-	-	-	-	-	-	-
No. Bolts	24	24	24	24	40	40	40	68	68







3038 AND 3030






3031 AND ABOVE







3031 & 3032

3033

3034 & 3035

3036 & 3037

Advanced Witness Systems Ltd © 2024

MANUFACTURER INFORMATION	SUPPLIER INFORMATION
Advanced Witness Systems Ltd	
Unit 8	
Beaumont Business Centre	
Beaumont Close	
Banbury	
OX16 1TN	
Tel: +44 (0)1295 266939	
Email: sales@awstorque.co.uk	
Catalogu	e Page 26

N-TYPE ROTARY TORQUE TRANSDUCER

DESCRIPTION

The AWS LTD N-type Rotary Torque Transducer range (NRTT), is designed to accurately measure torque values in a rotating shaft, in a variety of industries.

With optimised torque ranges, the transducer outputs a mV signal proportional to the supply voltage and torque. The transducer contains a memory chip in which a small selection of parameters, including serial number, model number, and calibration value, are held, compatible for setting some manufacturers display units.

The NRTT can be produced with different adapters depending on its use including square (standard) and keyway (option).

SPECIFICATIONS

Tel: +44 (0)1295 266939 Email: sales@awstorque.co.uk

Model: NRTT-	3041	3042	3043	3044	3045
Ranges:	0.4-10Nm	2-50Nm	10-250Nm	20-500Nm	40-1000Nm
Square Drive Size:	1/4"	3/ " /8	1/2"	3⁄4"	3⁄4"
Keyway Size:	Multiple sizes	Multiple sizes	Multiple sizes	Multiple sizes	Multiple sizes

Better than 0.1% of reading from 10 to 100% of rated output. See calibration

Accuracy:

certificate for full results. Signal Output: 2mV/V Communications: Not Applicable Bridge Impedance: 350Ω 10V DC 30mA Max Voltage and Current Requirement: Power and Display: Requires DC power supply and Dedicated mV meter Adapter: The NRTT can be produced with shaft ends suitable to its indented function. Speed: Standard 20,000 RPM Overload capability: 125% Maximum mechanical 160% of range stated. overload: **Operating Temperature:** -10°C to +50°C. Mil C 26482 series. Connector: 6 pin. Shell size 10. CE: 2014/30/EU EMC: BS EN 61326:2007 Advanced Witness Systems Ltd © 2024 MANUFACTURER INFORMATION SUPPLIER INFORMATION Advanced Witness Systems Ltd Unit 8 **Beaumont Business Centre Beaumont Close** Banbury OX16 1TN

> Data was correct at time of publication. Catalogue Page 27

DISPLAYS & BENCH TESTERS

Our Professional Transducer Display and Bench Testers use our unique inbuilt instrumentation PCBs to eliminate signal loss. Whether using one of our Intelligent Transducers, or a Bench Tester, the models accommodate your torque and budget requirements.

Displays & Bench Testers	PAGE
Professional Transducer Display	29
Professional Torque Tool Tester	30
Professional Calibration Torque Unit	31

Advanced Witness Systems Ltd Catalogue 2024 Data was correct at time of publication. Catalogue Page 28

PROFESSIONAL TRANSDUCER DISPLAY

DESCRIPTION

The PTD is designed for powering and displaying the readings from AWS Intelligent Torque Transducer ranges (I Series). The PTD features a bright, full colour LCD graphic display, showing the torque reading, both in large 6 digits, and analogue bar graph. The PTD features Run, Peak and 1st Peak mode operation, unit and limits selection via front *panel soft keys*. When using the limits features, external yellow, red and green LEDs indicate whether torque values are low, high or acceptable, and the 6 digit reading changes colour. The PTD displays torque in Nm, cNm, Lbf.Ft, Lbf.In and Ozf.In. RS232 output enables the PTD to be connected to a PC for direct input into ADMS Kepler 4 Calibration and Conformity Software (sold separately).

The 1010M is designed for use with the AWS UTWCM (Sold separately). The models 1010B and 1010H have internal rechargeable batteries for portable operation. These models also indicate the battery level status. The 1010H is a more rugged option for demanding environmental climates. The AWS Professional Transducer Display (PTD) is available in three versions: 1010M, 1010B and 1010H. All versions casings have a rugged solid design for withstanding shock & impact damage.

SPECIFICATIONS

Model: PTD-	1010M	1010B	1010-Н
Specification	Mains power supply from 12V DC charger.	Internal rechargeable batteries.	Internal rechargeable batteries. Heated display for use at sub-zero temperatures. Rated to IP 67.
LCD Display:	6 DigitAnalog	Active Reading ue Bar Graph	Sunlight Readable LCD Display
Power:	• Battery 1010M – 1010B/H	Unit, Limit Selection and Sett State and Indication of Char Mains powered from 12V DC - Internal Rechargeable Batte extends life of the display. Sup	ging (1010B/H). charger eries allow for portable use. Auto power off
Accuracy:	Better tha Transduc		100% F.S.D when used with AWS Intelligent Torque
Limit Selection:	Low, Pas	s, High	
Units:	Nm, cNm	n, LbfFt, LbfIn, OzfIn	
Data Output:		Standard Female Connector	
Operating tempera		: -10 to +50°C	
Temperature coef		20 to +50°C 0.01% per °C	
		: 0.03% per °C	
Mode:	RUN	PEAK	<u>→→→→→↓↓→→→↓</u> 57.98
Weight:	1.6 Kg		🗢 Mode Tare Reset
Size:	160mm >	220mm x 200mm	
CE:	2014/30/	EU	that had been set to be
EMC:	EN 6132	6-1:2013	
NATO Stock No: Screenshots:	5980-22-	623-1641	PROFESSIONAL TRANSDUCER DISPLAY
SELECT MODE			
Run First Peak	<u>}</u> ₪ 60.00)	
Left: Graphical mo	ок 🇢 ^{Моde} Tare	Reset PLEASE CONNECT CHARG	

Left: Graphical mode selection. Centre: Reading screen showing mod units selected and analogue bar graph. Right: Battery level warning

PROFESSIONAL TORQUE TOOL TESTER

DESCRIPTION

The AWS LTD Professional Torque Tool Tester range (PTTT), the companies' premier bench mounted tester range, for calibrating, testing and certifying hand torque tools.

The PTTT features a bright, full colour LCD graphic display, showing the torque reading, both in large 6 digits, and analogue bar graph. A flexible neck means the full colour display can be easily read from any position. It has internal rechargeable batteries for portable operation. Featuring Run, Peak and 1st Peak mode operation (selectable to allow use with all types of torque tool), unit and limits selection via front panel soft keys. When using the limits features, external yellow, red and green LEDs indicate whether torgue values are low, high or acceptable, and the 6 digit reading changes colour. The display also indicates the battery level status. The RS232 output enables the PTTT to be connected to a PC for direct input into ADMS Kepler Torque Tool Calibration Software (sold separately). This allows for quick, accurate and precise calibration of torque tools.

SPECIFICATIONS

Model: PTTT-1005-	10	50	250	1000
Ranges:	0.4 - 10Nm	2 - 50Nm	10 - 250Nm	40 - 1000Nm
Square Drive Size:	1/4"	3/8"	1/2"	3/4"

Better than 1% of reading from 4 to 100% of Rated output. See Calibration certificate for full Accuracy: results. Run: For Dial-type and Electronic Wrenches and Screwdrivers Modes: Peak: For Cam-type Wrenches and Screwdrivers. 1st Peak: For Click-type Wrenches and Screwdrivers, retains reading until manually cancelled or for 3 seconds if auto cancel option is chosen. 70mm X 52mm Bright Full Colour Sunlight Readable LCD Display of 6 Digit Active Reading, with LCD Display: Analogue Bar Graph, Mode Selection graphics, Battery State and indication of charging. Optional limit selection with colour indication shows whether a reading is Above Limit, Below Limit and Within Limit. All functions are selected and changed by soft keys. Internal Rechargeable Batteries allow it to be used in the field. Auto power off function extends life Power: of the display. Supplied with 12V DC power supply for charging batteries and mains power. Data Output: Female RS232 connection Overload capability: 125% Maximum mechanical 160% of Range stated. overload: +5°C to +50°C. IP67. Operating temperature: Temperature coefficient: On Zero: 0.01% per °C On Span: 0.03% per °C **Torque Standard:** BS 7882:2017 2014/30/EU CE NATO Stock No: PTTT-1005-50: 6625-22-623-1637 PTTT-1005-1000: 6625-22-623-16348 ScreenShots: SELECT MODE **BATTERY LEVEL** 123450

Mode Tare Reset \bigcirc Left: Graphical Mode selection. Centre: Reading Screen Showing mode/ units selected and Analogue Bar graph. Right: Battery level warning

A

OK



Advanced Witness Systems Ltd © 2024

MANUFACTURER INFORMATION
Advanced Witness Systems Ltd
Unit 8
Beaumont Business Centre
Beaumont Close
Banbury
OX16 1TN
Tel: +44 (0)1295 266939
Email: sales@awstorgue.co.uk

Data was correct at time of publication. Catalogue Page 30

PROFESSIONAL CALIBRATION TORQUE UNIT

DESCRIPTION

The AWS LTD Professional Calibration Torque Unit (PCTU), our entry level bench mounted tester for production line or lower cost requirements for testing hand torque tools.

With Multiple mode and unit selection as well as a tilting display providing a variety of viewing angles, it does not compromise on function or accuracy, displaying more precise torque values than any other entry level torque tool tester.

The range is designed to calibrate all types of torque wrenches and torque screwdrivers, and has been selected to cover the large majority of torque tools without having to use two instruments for a single tool type.

The RS232 output enables the PCTU to be connected to a PC for direct input into ADMS Kepler Torque Tool Calibration Software (sold separately). This allows for quick, accurate and precise calibration of torque tools.

SPECIFICATIONS

Model: PCTU-1006-	10	50	250	1000				
Ranges:	0.4 - 10Nm	2 - 50Nm	10 - 250Nm	40 - 1000Nm				
Square Drive Size:	1/4"	3/8"	1/2"	3/4"				
Accuracy:	Better than 1% of rear	ading from 4 to 100%	of Rated output. See Ca	libration certificate for full				
Units:	Nm and Lbf.Ft or cN	m and Lbf.In Selectat	le (Dependant on Range	e).				
Modes:	A 1st PEAK: For Click-	UN: For Dial-type and Electronic Wrenches and Screwdrivers st PEAK: For Click-type Wrenches and Screwdrivers EAK: For Cam-type Wrenches and Screwdrivers						
Display:	5 X 12.5mm digit LE	5 X 12.5mm digit LED. Adjustable viewing angle through 90°. LED's indicate selected mode and units. Selection and functions are changeable by four pushbuttons.						
Power:		Internal Rechargeable Batteries allow it to be used in the field. Auto power off function extends life of the display. Supplied with 9V DC plug top power supply for charging batteries and mains						
	power.							
Mounting:	Wall or bench/pedea	stal mountable via 4 h	ole 8 mm dia bolt fixings	(bolts not supplied).				
Data Output:	Female RS232 conr	ection.		_				
Overload capability:	125%		PROFESSIONAL CALIBR	ATION				
Maximum mechanical overload:	160% of Range state	ed.	ON DOMINIC	(neser)				
Operating temperature:	+0°C to +50°C.		A 00000					
Temperature coefficient:	On Zero: 0.01% per On Span: 0.03% per		C LA DA DO FILB NM ((tane)				
CE:	2014/30/EU							
EMC:	EN 61326: 2007							
Torque Standard:	BS 7882:2017		- Breine					

Advanced Witness Systems Ltd © 2024

MANUFACTURER INFORMATION

Advanced Witness Systems Ltd Unit 8 Beaumont Business Centre Beaumont Close Banbury OX16 1TN Tel: +44 (0)1295 266939 Email: sales@awstorque.co.uk

SUPPLIER INFORMATION

Data was correct at time of publication. Catalogue Page 31

TRANSDUCER ANCILLARIES

A selection of products which can be used with AWS Transducers, Displays and Bench Testers, and also in association with other manufacturers Transducers & Displays.

Transducer Ancillaries	PAGE
Precision Torque Adapters	33-34
Multiway Transducer Switch Box	35
Intelligent Instrument Transducer Cable	36
Transducer Cables	37

Advanced Witness Systems Ltd Catalogue 2024 Data was correct at time of publication. Catalogue Page 32

PRECISION TORQUE ADAPTERS

Hex-Square Adapters

DESCRIPTION

The AWS LTD Precision Torque Adapters, designed to improve the accuracy and reduce the uncertainty in torque calibration & apparatus. Our precision adapters cover a range of the most commonly used square drive, hex and keyway sizes. Keyways can be produced to specific standard as well as non-standard sizes. Because of this they can be used on a variety of different calibration machines and apparatus. They are manufactured to high tolerances out of hardened stainless steel to eliminate corrosion and increase the lifetime of the adapters. They are laser engraved with the size and model number for easy identification.

Part No:				Siz	e:		
CM105	1"	F	SQ	to	36mm	F	HEX
CM150	1"	F	SQ	to	1⁄4"	F	HEX
CM151	1"	F	SQ	to	6mm	F	HEX
CM152	1"	F	SQ	to	10mm	F	HEX
CM153	1"	F	SQ	to	17mm	F	HEX
CM154	1"	F	SQ	to	19mm	F	HEX
CM155	1"	F	SQ	to	22mm	F	HEX
CM156	1"	F	SQ	to	27mm	F	HEX
CM106	3⁄4"	F	SQ	to	36mm	F	HEX
CM113	3⁄4"	F	SQ	to	19mm	F	HEX
CM191	1⁄2"	F	SQ	to	1⁄4"	Μ	HEX
CM191	1⁄2"	F	SQ	to	1⁄4"	F	HEX
CM107	1⁄2"	F	SQ	to	19mm	F	HEX

Part No:	Size:						
CM111	1⁄2"	F	SQ	to	17mm	F	HEX
CM112	3/8"	F	SQ	to	19mm	F	HEX
CM110	3/8"	F	SQ	to	17mm	F	HEX
CM109	3/8"	F	SQ	to	10mm	F	HEX
CM171	3/8"	Μ	SQ	to	1⁄4"	F	HEX
CM172	3/8"	Μ	SQ	to	1⁄4"	М	HEX
CM108	1⁄4"	F	SQ	to	10mm	F	HEX
CM170	1⁄4"	Μ	SQ	to	1⁄4"	F	HEX
CM173	1⁄4"	Μ	SQ	to	1⁄4"	Μ	HEX
CM176	1⁄4"	F	SQ	to	1⁄4"	Μ	HEX
CM195	1⁄4"	F	SQ	to	1⁄4"	F	HEX
CM182	4mm	F	SQ	to	1⁄4"	F	HEX

Keyway-Square Adapters

Part No:	Size:						
CM138	1"	F	SQ	to	35mm	F	KEY
CM137	3⁄4''	F	SQ	to	35mm	F	KEY
CM136	1⁄2"	F	SQ	to	35mm	F	KEY
CM175	1⁄2"	F	SQ	to	20mm	F	KEY





Advanced Witness Systems Ltd © 2024 Data was correct at time of publication. Catalogue Page 33

Square-Square Adapters

Specifications

Part No:				Size:			
CM187	3.5"	F	SQ	to	3.5"	F	SQ
CM188	3.5"	Μ	SQ	to	2.5"	F	SQ
CM183	1.5"	Μ	SQ	to	1"	F	SQ
CM174	1.5"	Μ	SQ	to	³∕4″	F	SQ
CM184	1⁄2"	F	SQ	to	1⁄2"	F	SQ
CM132	1/2"	F	SQ	to	3/8"	F	SQ
CM139	3/8"	F	SQ	to	3/8"	F	SQ
CM141	1⁄4"	F	SQ	to	3/8"	F	SQ
CM140	1⁄4"	F	SQ	to	1⁄4"	F	SQ

CM190	3.5"	Μ	SQ	to	3.5"	Μ	SQ
CM189	3.5"	Μ	SQ	to	2.5"	Μ	SQ
CM142	1"	F	SQ	to	1.5"	Μ	SQ
CM177	1"	Μ	SQ	to	1"	Μ	SQ
CM146	1"	F	SQ	to	3⁄4"	Μ	SQ
CM178	1"	Μ	SQ	to	³∕4″	Μ	SQ
CM147	1"	F	SQ	to	1⁄2"	Μ	SQ
CM179	1"	Μ	SQ	to	1⁄2"	Μ	SQ
CM148	1"	F	SQ	to	3/8"	М	SQ
CM180	1"	Μ	SQ	to	3/8"	Μ	SQ

Part No:				Size:			
CM149	1"	F	SQ	to	1⁄4"	М	SQ
CM181	1"	Μ	SQ	to	1⁄4"	М	SQ
CM186	3⁄4"	Μ	SQ	to	1 5/8"	Μ	SQ
CM143	3⁄4"	F	SQ	to	1"	М	SQ
CM164	3⁄4"	F	SQ	to	1⁄2"	М	SQ
CM165	3⁄4"	F	SQ	to	3/8"	М	SQ
CM166	3⁄4"	F	SQ	to	1⁄4"	М	SQ
CM144	1⁄2"	F	SQ	to	1"	Μ	SQ
CM160	1⁄2"	F	SQ	to	3⁄4"	М	SQ
CM167	1⁄2"	F	SQ	to	3/8"	Μ	SQ
CM185	1⁄2"	Μ	SQ	to	3/8"	Μ	SQ
CM168	1⁄2"	F	SQ	to	1⁄4"	М	SQ
CM145	3/8"	F	SQ	to	1"	М	SQ
CM159	3/8"	F	SQ	to	3⁄4"	М	SQ
CM162	3/8"	F	SQ	to	1⁄2"	М	SQ
CM169	3/8"	F	SQ	to	1⁄4"	Μ	SQ
CM157	1⁄4"	F	SQ	to	1"	М	SQ
CM158	1⁄4"	F	SQ	to	3⁄4"	М	SQ
CM161	1⁄4"	F	SQ	to	1⁄2"	Μ	SQ
CM163	1⁄4"	F	SQ	to	3/8"	Μ	SQ

Annular Transducer Mounting Adapters

The AWS LTD Annular Transducer Mounting Adapters, which are bespoke designed to fit any mounting arrangement, and designed to improve the accuracy of calibration results. They can be used to turn one of our high torque Annular Transducers into a high torque Inline Transducer. They are manufactured to high tolerances out of hardened stainless steel to eliminate corrosion and increase the lifetime of the adapters. They are laser engraved with the size and model number for easy identification.

Unique Custom-Design Adapters

AWS LTD can custom design & manufacture unique high tolerance adapters for customers who require something specific that is not part of our range. These will be designed & checked to meet the customers' specification, manufactured to high tolerances, and plated to eliminate corrosion and increase the lifetime of the adapters. They are laser engraved with the size and custom model number for easy identification.

MANUFACTURER INFORMATION	SUPPLIER INFORMATION				
Advanced Witness Systems Ltd					
Unit 8					
Beaumont Business Centre					
Beaumont Close					
Banbury					
OX16 1TN					
Tel: +44 (0)1295 266939					
Email: sales@awstorgue.co.uk					

Advanced Witness Systems Ltd © 2024

MULTI-WAY TRANSDUCER SWITCH BOX



DESCRIPTION

The AWS Ltd Multiway Transducer Switch Box (TSB) is designed to be used with the AWS Universal Torque Wrench Calibration Machine (UTWCM) and Professional Transducer Display (PTD). It switches between and provides continuous power (for thermal stability) to a number of AWS Intelligent Torque Transducers or Intelligent Instrumented Transducer Cables.

The Transducer Switch Box simultaneously powers the multiple transducers and the Professional Transducer Display. There are connectors on the back for RS232 output to a PC, and for communication with the PTD and UTWCM.

The PTD is connected to the TSB via a single cable, which connects to the Auxiliary port on the Display. The RS232 output data is generated by the PTD. The UTWCM is also connected to the TSB via a single cable, allowing the UTWCM to be run in automatic operation.

Specification

Power:	Mains powered from 12V DC charger
Inputs:	4/6 off 6 Way Mil C Spec connectors
Outputs:	3 off 9-pin D Standard Female Connector:
	RS232 Output
	1010 Display
	UTWCM
Size:	17cm x 11cm x 9cm
Weight:	0.5 Kg



Model	1057-4	1057-6
Number of Transducers	4	6

Cables to use with the TSB can be supplied depending on specific customer requirements.

INTELLIGENT INSTRUMENTED TORQUE TRANSDUCER CABLE



The AWS LTD Intelligent Instrumented Torque Transducer Cable (IITC), is designed to convert standard mV/V transducers from any manufacturer into truly intelligent digital transducers.

The cable contains our Intelligent Instrumentation Package, outputting using CAN-BUS protocol to communicate with the AWS LTD Professional Transducer Display (PTD). This digital communication eliminates signal loss when using long lengths of cable, providing flexibility in communicating with other devices and systems.

A simple 2 step calibration.

Stores serial & model number, capacity, calibration coefficient, units of calibration, and conversion to other torque units.

Each cable is calibrated only to a specific dedicated transducer, remaining unique to that transducer.

Modes: Communications: Power and Display: Connector: 

Communications via can bus. (When used with the AWS PTD-1010 power & display unit). D.C power supply (When used with AWS PTD-1010, power and display is provided). Mil C 26482 series to Mil C 26482 series. 6 pin. Shell size 10.

Model: IITC-1008-	1	2	5	10
Length:	1m	2m	5m	10m



Advanced Witness Systems Ltd © 2024

MANUFACTURER INFORMATION
Advanced Witness Systems Ltd
Unit 8
Beaumont Business Centre
Beaumont Close
Banbury
OX16 1TN
Tel: +44 (0)1295 266939
Email: sales@awstorgue.co.uk

SUPPLIER INFORMATION

Intelligent Torque Transducer Connector Cable

The AWS LTD Intelligent Torque Transducer Cable (ITC), used to connect any AWS LTD Intelligent (I Series) Transducer to the AWS LTD Professional Transducer Display (PTD). It has a female MIL C connector transducer-end, and a male MIL C connector display-end. These cables come in a selection of standard lengths, or if a specific length is required, we will manufacture one to specification.

Model: ITC-1009-	1	2	5	10
Length:	1m	2m	5m	10m



N-SERIES Torque Transducer Cable

The AWS LTD N-SERIES Torque Transducer Cable range (NTC), our basic cable for connecting our A SERIES and N SERIES transducers to other manufacturers displays which use MIL-C or LEMO connectors for signal input. These cables come in a selection of standard lengths, or if a specific length is required, we will manufacture one to specification.

Model: NTC-	2008	2009	2010
Female Connector:	6 Pin MIL-C	6 Pin MIL-C	10 Pin MIL-C
Male Connector:	6 Pin MIL-C	10 Pin LEMO	10 Pin LEMO

These cables come in a selection of standard lengths, or if a specific length is required, we will manufacture to specification.

Model: NTC-20##-	1	2	5	10
Length:	1m	2m	5m	10m

Advanced Witness Systems Ltd © 2024

MANUFACTURER INFORMATION	SUPPLIER INFORMATION
Advanced Witness Systems Ltd	
Unit 8	
Beaumont Business Centre	
Beaumont Close	
Banbury	
OX16 1TN	
Tel: +44 (0)1295 266939	
Email: sales@awstorgue.co.uk	

CALIBRATION MACHINES

Our Torque Calibration Machines are for calibrating Torque Tools and Transducers to the latest International Torque Standards.

Calibration Machines	PAGE
Universal Torque Wrench Calibration Machine	39-40
What Creates the UTWCM	41
UTWCM Return on Investment	42
Universal Torque Screwdriver Calibration Machine	43-44
UTSCM Handle Adapters	45-46
What Creates the UTSCM	47
UTSCM Return on Investment	48
Universal Torque Calibration Machine	49-50
Unsupported Calibration Beams	51-53
2Nm Calibration Machine	54

UNIVERSAL

TORQUE WRENCH CALIBRATION MACHINE



Photo above shows a UTWCM with AWS Intelligent Inline Torque Transducers, Professional Transducer Display, and Laptop/Computer running ADMS Kepler 4 Software for Calibration & Conformity to ISO 6789:2017 Parts 1 and 2.

DESCRIPTION

The all new AWS Universal Torque Wrench Calibration Machine (UTWCM) provides an efficient means of calibrating and testing manually operated torque wrenches to ISO 6789:2017, ISO 6789:2003 or company specific standards and specifications.

The UTWCM is available in 6 versions; Automated or Semi-automated operation and ranges up to either 500Nm, 1500Nm or 3000Nm. All versions apply the force to the tool via a linear carriage stepper motor and an AWS microcontroller. An important feature is the minimization of parasitic forces applied to the torque wrench handle, due to the method of mounting the torque wrench. All versions of the machine can be used with our new ADMS Kepler 4 software to speed up completion of the calibration & certification process to ISO 6789:2017, ISO 6789:2003 or type approval for manufacturers.

The automated UTWCM uses AWS Intelligent Inline Torque Transducers (IITT's) and a Professional Transducer Display (PTD) to provide feedback to the microcontroller, automatically detecting a first peak signal for setting type wrenches, stopping the machine and returning to zero, greatly speeding up the calibration process and reducing operator input.

The semi-automated UTWCM, using its push buttons, controls the force on the tool. It relies on the operator to detect the target torque and stop the machine.

Specification

Model: UTWCM -	500 - S	500 - A	1500 - S	1500 - A	3000 - S	3000 - A
Range:	500 Nm	500 Nm	1500 Nm	1500 Nm	3000 Nm	3000 Nm
Manual or Semi- Automated:	Semi- Automated	Automated	Semi - Automated	Automated	Semi - Automated	Automated

Shared Features

- Designed to calibrate/test wrenches up to either 500, 1,500 or 3,000 N·m.
- The 500Nm version of the AWS Universal Torque Wrench Calibration Machine can be desktop mounted, meaning it requires less footprint to house the machine.

- Removes the need for operators to apply high application forces to the handle of large torque wrenches. Force is applied using inbuilt AWS proprietary firmware, a stepper motor and linear track system.
- Hand controls for fast movement or jog facilitate quick setting up of individual wrenches.
- Multiple safety features ensure that the machine, transducers and torque wrench are not overloaded in operation or over driven due to a wrench fault.
- Inbuilt microcontroller for accurate control of force applied and operation speeds. Four different pre-programmed, switch selected speed settings for different ranges of tools. The microcontroller ensures the adherence to the minimum target torque approach times, complying with the ISO standard 6789:2017, for the capacity of wrench being calibrated.
- Parasitic forces acting on the wrench during calibration are greatly reduced by the method of mounting the torque wrench.



UTWCM with 60N·m Torque Wrench

- Multiple or single transducer cassette variations for different transducer manufacturers are available or built to suit customer requirements.
- To accommodate wrenches with fixed heads the transducer can be rotated 360 ° in steps of 30°.

AUTOMATED FEATURES

• A Customer's existing transducers can be converted into IITTs using AWS's Intelligent Instrumented Transducer Cables. Each cable has an inline module converting the analogue output of the transducer into a digital torque signal for display on the PTD.



Simple and Intuitive Handheld Controller

- Connecting an AWS IITT automatically programs the AWS PTD to the correct range.
- When operating the AWS PTD in First Peak mode for click wrenches, the machine will run a complete operation cycle automatically.

DIMENSIONS

Dimensions for mounting on floor:

UTWCM-500: Approx. 110cm W by 90cm H. Requires desk space of 75cm D by 70cm W. Overhangs front of desk by 45cm, and requires 56cm of space above the table.

UTWCM-1500: Approx. 77cm D by 205cm W by 135cm H. Footprint is approx. 77cm D by 165cm W.

UTWCM-3000: Approx. 77cm D by 266cm W by 135cm H. Footprint is approx. 77cm D by 165cm W.

Depth, Width and Height can be altered if required within certain parameters.

More information on the Intelligent Inline Torque Transducers range, Professional Transducer Display and Kepler 4 software is available in separate data sheets on the AWS website www.awstorque.co.uk.

Advanced Witness Systems Ltd © 2024 | ® 6169133 | ® 6169134

SUPPLIER INFORMATION


MANUFACTURER INFORMATION Advanced Witness Systems Ltd Unit 8 Beaumont Business Centre Beaumont Close Banbury OX16 1TN Tel: +44 (0)1295 266939 Email: sales@awstorque.co.uk



Advanced Witness Systems Ltd.

Unit 8 Beaumont Business Centre, Banbury. OX16 1TN Tel: +44 (0) 1295 266939 e-mail: sales@awstorque.co.uk Head Office: 1st Floor, No 1 Carrera House, Merlin Court, Gatehouse Close, Aylesbury, Buckinghamshire, HP19 8DP

WHAT CREATES THE UNIVERSAL TORQUE WRENCH CALIBRATION MACHINE:

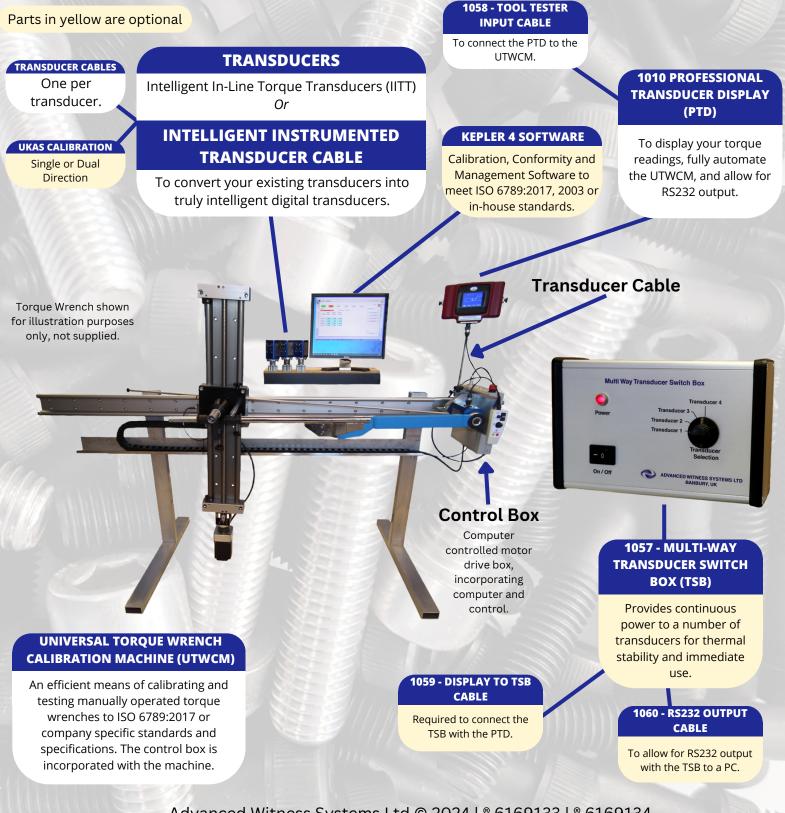

Advanced Witness Systems Ltd © 2024 | [®] 6169133 | [®] 6169134 Data was correct at time of publication. Catalogue Page 41



CALIBRATE 3X FASTER WITH THE AWS

UNIVERSAL TORQUE WRENCH CALIBRATION MACHINE

We set out below the real major cost, time and operator advantages against manual operation, with typical proven examples.

About the Universal Torque Wrench Calibration Machine

The AWS Universal Torque Wrench Calibration Machine (UTWCM) for calibrating and testing manually operated torque wrenches to ISO 6789:2017, ISO 6789:2003 or company specific standards. Available in 2 versions, 1.5kN-m or 3kN-m, it removes the requirements for operators applying high application forces to the handle of large torque wrenches. The inbuilt microcontroller accurately controls the force applied and the operational speeds. This ensures the adherence to the minimum target torque approach times, complying with ISO 6789:2017. Parasitic forces are reduced to minimal levels by the method of mounting and controlling the applied force. It can be used with our Kepler 4 software to further increase productivity, eliminate data entry errors, comply with ISO 6789:2017 & 2003, and produce certificates.

Return on Investment – ISO 6789:2017:

- Users already meeting ISO 6789:2017 by manual means find it is very time consuming and requires quite some skill and operator effort, typically requiring an oscilloscope for checking the final 20% of the applied torque is below the timing requirement set out in the standard.
- Time taken can be up to an hour and a half, and very dependent on operator skill.
- Using the AWS UTWCM, typical calibration time is <u>60 minutes</u>, and with much less operator skill & effort.
- Considerable time saving, generating faster throughput of torque wrenches.
- Using the AWS UTWCM is <u>1/3 quicker</u> than the manual method.
- Payback can be as short as <u>6 months*</u>.

Original Calibration Time	90 mins
New Calibration Time	60 mins
Payback	6 months*

Return on Investment – ISO 6789:2003:

- Using the AWS UTWCM to meet ISO 6789:2003, typical calibration time is only 20 minutes.
- Using the UTWCM is <u>3 times faster</u>, increasing throughput and reducing errors, with less operator skill.
- Payback estimated to be as short as <u>6 months**</u>.

Typical timings for the various calibrations are shown overleaf. *Based on approximate cost of UTWCM, 6 calibrations

Original Calibration Time	60 mins
Calibration Time with UTWCM	20 mins
Payback	6 months**

*Based on approximate cost of UTWCM, 6 calibration per day, £35/hour hourly rate. **Based on approximate cost of UTWCM, 12 calibrations per day, £35/hour hourly rate.

Advanced Witness Systems Ltd © 2024 | ® 6169133 | ® 6169134

Advanced Witness Systems Ltd
Unit 8
Beaumont Business Centre
Beaumont Close
Banbury
OX16 1TN
Tel: +44 (0)1295 266939
Email: sales@awstorque.co.uk

UNIVERSAL TORQUE SCREWDRIVER CALIBRATION MACHINE



Photo above shows a UTSCM with Control Box, Handheld Controller, and an Intelligent Inline Torque Transducer.

DESCRIPTION

The all new AWS Universal Torque Screwdriver Calibration Machine (UTSCM) for compliance to ISO 6789:2017 provides an efficient means of calibrating and testing manually operated torque screwdrivers to international or company specific standards and specifications.

The UTSCM applies torque to the screwdriver via a tooth belt drive and an AWS microcontroller, the torque achieved is measured by 1 of 3 AWS Intelligent Inline Torque Transducers (IITT's), connected to an in-built Professional Transducer Display to automatically detect a peak signal.

The UTSCM can be used with our new ADMS Kepler 4 software to speed up completion of the calibration & certification process to ISO 6789:2017, 2003 or type approval for manufacturers.


With the variation in torque screwdriver operation, the UTSCM using a microcontroller, runs through a learning cycle before calibration to record the shape of the torque curve, ensuring the torque is applied at the correct rate meeting the ISO standard. As required by the standard, the number of operations are selectable, capturing each reading consecutively, greatly reducing the time for the calibration & certification process.

Due to the great variation in screwdriver handles, grip adaptors are bespoke designed to fit a specific model. This to minimise the uncertainty of torque screwdriver alignment, ensuring it is within $\pm 2^{\circ}$ of vertical alignment, as required by the standard.

FEATURES

- Designed to calibrate/test screwdrivers up to 30 N·m.
- Inbuilt microcontroller and display for accurate control of torque applied and operational speed. The microcontroller learns the shape of the torque curve, ensures adherence to the minimum and maximum target torque approach times, complying with the ISO standard, for the setting of the screwdriver being calibrated.
- The screwdriver type can be selected, to be either cam, dial (indicating) or click type.

- Auto operation meaning the number of consecutive operations can be selected, either 1, 3, 5 or 10 as required by the standard and then started with the push of a button.
- An in-built 3-Way Transducer Switch Box keeps the AWS Intelligent Transducers powered continually, aiding temperature stability. This allows quick selection of transducers. The controller automatically interrogates and displays the correct transducer range.
- Interchangeable handle adaptors each designed to accurately fit the model of torque screwdriver to minimise the uncertainty of adaptor alignment and ensure the screwdriver is within ± 2° of vertical.
- Height adjustable transducer carriage taking into account varying torque screwdriver lengths.
- Pendant control for fast movement or jog facilitate quick calibration set up of individual screwdrivers.
- Safety features ensure that the machine, transducers and screwdriver are not overloaded in operation or over driven due to a fault.
- 3/8"- 1/4" female square drive compatible with a range of torque transducers.
- A customer's existing transducers may be converted into IITTs using AWS's Intelligent Instrumented Transducer Cables. Each cable has an inline module converting the analogue output of the transducer into a digital torque signal for display on the PTD.
- 70mm X 52mm Bright, Full Colour, Sunlight Readable LCD Display built into the microcontroller.
- Soft keys, in conjunction with the graphics, allow selection of the required Mode, Measurement Unit, and Limit Selections.
- Active 6 Digit display. Accuracy better than 1% of reading from 4% to 100% full scale deflection of the selected transducer when used with AWS Intelligent Torque Transducers.
- For viewing difficult to read indicating type screwdrivers, an optional flexible probe camera with a built in display is available.

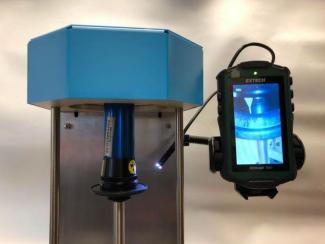

DIMENSIONS

Photo above shows a UTSCM in use with the optional flexible probe camera, showing a view of the dial on its in-built display.

Dimensions for mounting on benches/ tables: Approximately 31cm L by 45cm W by 45cm H.

UTSCM Weight: 16.5kg with an AWS IITT transducer, Control Box Weight: 5kg

More information on the Intelligent Inline Torque Transducers range and Kepler 4 software is available in separate data sheets on the AWS website www.awstorque.co.uk.				
Advanced Witness Systems Ltd	d © 2024 ® 6169127 ® 6169130			
MANUFACTURER INFORMATION Advanced Witness Systems Ltd Unit 8 Beaumont Business Centre Beaumont Close Banbury OX16 1TN Tel: +44 (0)1295 266939 Email: sales@awstorque.co.uk	SUPPLIER INFORMATION			
Email: sales@awstorque.co.uk Data was correct at time of publication.				

Catalogue Page 44

UTSCM SCREWDRIVER HANDLE Adapters



Photo above shows various AWS solid torque screwdriver handle adapters.

DESCRIPTION

The all new AWS Universal Torque Screwdriver Calibration Machine (UTSCM) for compliance to ISO 6789:2017 provides an efficient means of calibrating and testing manually operated torque screwdrivers to international or company specific standards and specifications.

There are numerous screwdriver handle designs which AWS have addressed for this machine with a range of adapters available for the UTSCM. Solid Adapters grip one specific model of torque screwdriver. Square Drive and Adjustable Adapters are designed to accommodate a variety of different torque screwdriver models.

All types of adapters comply fully with the ISO 6789:2017 Part 1 requirement that the torque screwdriver must be held within $\pm 2^{\circ}$ of vertical.

Adapters for models of torque screwdrivers not listed are available on request.

SOLID ADAPTER FEATURES

- 30Nm rated torque.
- Accurate fitting of a specific model of torque screwdriver handle.
- Simple design for easy interchangeability.
- Produced in specialised plastics for strength and fatigue life.

Adjustable Adapter Features

- 10Nm rated torque.
- Produced in specialised plastics for strength and fatigue life.
- Chuck / collet hybrid design accommodates a wide range of torque screwdriver models.
- Adapts to knurled, fluted and a variety of cushion grip handles.
- Simple to switch between different screwdriver models for fast turnaround time.
- A set of flexible knurled Top Hats included for gripping more difficult torque screwdriver shapes while retaining tool surface finish.
- Easy tightening and untightening of the adapter using included tool.





Advanced Witness Systems Ltd © 2024 | ® 6169131 | ® 6169132 Data was correct at time of publication. Catalogue Page 45

SQUARE DRIVE ADAPTER FEATURES

- 30Nm rated torque.
- 1/4" Male Square drive adapter.
- Aluminium construction with precision square drive.

LIST OF AVALIABLE ADAPTERS

Solid Adapters

For solid adapters for a specific manufacture's model of torque screwdriver, please contact AWS stating the screwdriver model.

Square Drive Adapters

Adapter Model	Torque Range	Handle Diameter Range	Drive	Screwdriver Model
2040-ASQ1	0-30Nm	N/A	1/4" Male SQ	Various

Adjustable Adapters

Adapter	Torque	Handle	Number of	Flexible	Screwdriver
Model	Range	Diameter	teeth	Knurled Top	Model
		Range		Hat Sizes	
2040-AA1	0-10Nm	15mm -36mm	4	20mm ID	Various
				27mm ID	
				34mm ID	
2040-AA2	0-10Nm	30mm-45mm	4	38mm ID	Various
				45mm ID	

Please note: AWS has researched a wide variety of torque screwdriver shapes and sizes. Our adapters grip an extensive range of torque screwdriver handles however there may be a particular that we have not been able to research. If in doubt please contact

AWS.

Advanced Witness Systems Ltd © 2024 ® 6169131 ® 6169132					
MANUFACTURER INFORMATION	SUPPLIER INFORMATION				
Advanced Witness Systems Ltd					
Unit 8					
Beaumont Business Centre					
Beaumont Close					
Banbury					
OX16 1TN					
Tel: +44 (0)1295 266939					
Email: sales@awstorque.co.uk					



Advanced Witness Systems Ltd.

Unit 8 Beaumont Business Centre, Banbury. OX16 1TN Tel: +44 (0) 1295 266939 e-mail: sales@awstorque.co.uk Head Office: 1st Floor, No 1 Carrera House, Merlin Court, Gatehouse Close, Aylesbury, Buckinghamshire, HP19 8DP

WHAT CREATES THE UNIVERSAL TORQUE SCREWDRIVER CALIBRATION MACHINE:



Catalogue Page 47



CALIBRATE 10X FASTER WITH THE AWS

UNIVERSAL TORQUE SCREWDRIVER CALIBRATION MACHINE

We set out below the real major cost, time and operator advantages against manual operation, with typical proven examples.

About the Universal Torque Screwdriver Calibration Machine

The all new AWS Universal Torque Screwdriver Calibration Machine (UTSCM), for calibrating and testing manually operated torque screwdrivers to ISO 6789:2017, ISO 6789:2003 or company specific standards. Designed to calibrate or test all known types, makes & models of torque screwdrivers and torque watches up to 30 Nm. The number of consecutive operations can be selected as required by the standard. Interchangeable handle adapters are designed to accommodate various models of torque screwdriver, minimising uncertainty. The microcontroller performs a learning cycle before calibration, recording the shape of the tool's torque curve, ensuring the correct rate of the applied torque meets the ISO standard. The UTSCM can be used with our Kepler 4 software to further increase productivity and eliminate data entry errors.

Return on Investment – ISO 6789:2017:

- Users already meeting ISO 6789:2017 by manual means find it is very time consuming and requires quite some skill, typically requiring an oscilloscope for checking the final 20% of the applied torque is within the 0.5-1 second required by the standard.
- Time taken can be up to 4 hours, and very dependent on operator skill.
- Using the AWS UTSCM, example calibration time is <u>25 minutes</u>, and with much less operator skill.
- Considerable time saving, generating faster throughput of torque screwdrivers.
- Using the AWS UTSCM is <u>10 times faster</u> than the manual method.
- Payback can be as short as a phenomenal <u>10 days*</u>.

Original Calibration Time	240 mins
Calibration Time with UTSCM	25 mins
Payback	10 days*

Return on Investment – ISO 6789:2003:

- Using the AWS UTSCM to meet ISO 6789:2003, example calibration time is only 7 minutes.
- Using the UTSCM is <u>6 times faster</u>, increasing throughput and reducing errors, with less operator skill.
- Payback estimated to be as short as <u>6 weeks**</u>.


Original Calibration Time	45 mins
Calibration Time with UTSCM	7 mins
Payback	6 weeks**

Typical timings for the various calibrations are shown overleaf.

*Based on approximate cost of UTSCM & 3 transducers, 12 calibrations per day, £35/hour hourly rate. **Based on approximate cost of UTSCM & 3 transducers, 24 calibrations per day, £35/hour hourly rate.

Advanced Witness Systems Ltd © 2024 ® 6169127 ® 6169130					
MANUFACTURER INFORMATION	SUPPLIER INFORMATION				
Advanced Witness Systems Ltd					
Unit 8					
Beaumont Business Centre					
Beaumont Close					
Banbury					
OX16 1TN					
Tel: +44 (0)1295 266939					
Email: sales@awstorque.co.uk					

2KNM UNIVERSAL TORQUE CALIBRATION MACHINE

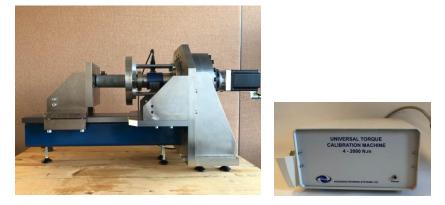

Bench mounted machine with Torque Transducer Sliding Carriage and 2kNm Master Transducer, alongside the control box.

Description


The AWS 4Nm-2000Nm Universal Torque Calibration Machine (3020-UTCM) is designed to provide a compact, efficient way to calibrate torque measuring devices to BS EN 7882:2017, BS EN:7996:2018 or international standards without the need for beams and weights. The machine uses two AWS Master Transducers (2000Nm and 100Nm) with very high accuracy, stability and low uncertainty. The master transducers output to an extremely accurate 7.5 digit computing digital voltmeter to display the applied torque and to attain the required uncertainty of measurement (Certificate of calibration provided).

The UTCM uses a high ratio anti backlash gearbox and stepper motor drive to apply and hold up to 2kNm torque. This is controlled by a pushbutton pendant controller removing the need for the operator to apply weights altogether (eliminating operator fatigue) and speeding up the calibration.

An additional Torque Tester Extension carriage with horizontal or additionally vertical fittings or mounting plate for a variety of torque measuring devices is available as an option (Sold Separately).

FEATURES

- Electronic drive system and push button pendant control, eliminating the need for the operator to manually apply torque.
- Unique drive system to remove parasitic forces ensuring full applied torque.
- Easily interchangeable inline master transducers for high accuracy and low uncertainty readings of the nominal torque. Range from 4 Nm to 2kNm.
- High ratio anti-backlash gearbox for precise torque application.

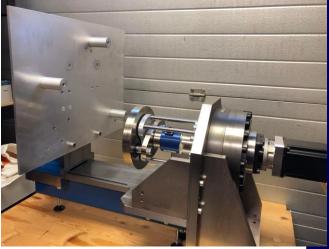

UTCM with Tool Tester Extension and Vertical Mounted Torque Tester fittings.

- Greatly reduced calibration times.
- Sliding carriage for calibration of standard sized torque transducers up to a 1" square drive.
- Bench or Pedestal mounting options available.
- Optional additional sliding carriage and fittings or mounting plate for calibration of a wide variety of torque measuring and calibration devices. Multi-axis T slot system and/or mounting plate for pick up of a range of fixing positions.

Advanced Witness Systems Ltd © 2024 | ® 6169128 Data was correct at time of publication. Catalogue Page 49

- Use with AWS Precision Torque Adapters each designed to accurately fit the model of torque testing device, minimising the uncertainty of adapter alignment.
- Additional alternative bed positions for vertical height adjustment, covering the wide variety of torque measuring devices available.
- High accuracy 7½ digit meter used to display the nominal torque readout from the master transducers to attain the required uncertainty of measurement.
- Jog function to precisely apply small increments of torque.
- The torque applied by the UTCM is indicated by a computing nano-voltmeter converting to units of torque from the mV/V signal from the transducer. A stable voltage source energises the transducers.



Torque Tester Extension with fittings for horizontal mount Torque Testers. AWS PTTT shown as device under test. (Sold separately)

The 7.5 digit computing nanovoltmeter and power supply to be used with the UTCM.



OPTIONS

		Options			
_	3020 - Universal Torque Calibration machine (UTCM)	Tool Tester Extension	Vertical Mounting Extension (Requires Tool Tester Extension)		
Model No.	3020	3020-Е	3020-EV		
Description	Calibration of torque transducers from 4Nm-2000Nm with square drives from ¼" to 1".	Additional fittings for calibration of vertical and horizontal mounting Torque Testers.	Additional fittings for calibration of large vertical or wall mounted Torque Testers.		

DIMENSIONS

Approx. dimensions for mounting on benches/tables: 94cm (length) x 34cm (width) x 40cm (height) Approx. Weight (Kg):

Main Body
(Without Transducers & Carriages)Transducer Sliding
CarriageTorque Tester Sliding Carriage
(Depending on options)103.516.724 - 40.5

Advanced Witness Systems Ltd © 2024 ® 6169128					
MANUFACTURER INFORMATION	SUPPLIER INFORMATION				
Advanced Witness Systems Ltd					
Unit 8					
Beaumont Business Centre					
Beaumont Close					
Banbury					
OX16 1TN					
Tel: +44 (0)1295 266939					
Email: sales@awstorgue.co.uk					

UNSUPPORTED CALIBRATION BEAMS



DESCRIPTION

The AWS Unsupported Calibration Beams are designed for calibration of torque measuring devices from 2 Nm - 1500 Nm using the principle of weights at a known distance. The beams are robust, precision machined anodised aluminium alloy components, and include a precision 1" (25.4mm) female square drive machined into the boss, to fit a selection of 1" (25.4mm) male to male adapters, allowing the beams to be used with AWS Precision Torque Adapters down to 1/4" in size, which facilitates a variety of devices to be calibrated. The calibration beams use kg weights. Precision weight pans, very flexible suspension cables, suspension hooks and a robust carry case are included. A UKAS calibration is available on request.

SPECIFICATION

- Uncertainty of Measurement better than 0.045% of reading.
- Female 1" Square Drive allows a selection of precision Male-Male adapters to be used as required (see table below)
- Cable, hooks and precision weight pans included.
- Designed to be used with kg weights.
- UKAS calibration available on request.

DIMENSIONS



Pedestal Available Separately

Useable Arc: 8 degrees For adequate clearance, use pedestal of 1.2m

Model: UCB-	3022	3023	3024	3025
Maximum Torque:	1500Nm	500Nm	50Nm	1000Lbf.Ft
Diameter:	2039mm	1019mm	510mm	1219mm
Height:	500mm	150mm	130mm	310mm

Precision Torque Adapter:				Size:			
CM177	1"	М	SQ	to	1"	М	SQ
CM178	1"	М	SQ	to	3⁄4″	Μ	SQ
CM179	1"	М	SQ	to	1⁄2"	М	SQ
CM180	1"	М	SQ	to	³∕8″	М	SQ
CM181	1"	М	SQ	to	1⁄4"	М	SQ

Advanced Witness Systems Ltd © 2024 Data was correct at time of publication. Catalogue Page 51

2NM UNSUPPORTED CALIBRATION WHEEL



DESCRIPTION

The AWS LTD 2Nm Unsupported Calibration Wheel is designed for calibration of torque measuring devices from 0.04Nm - 2 Nm using the principle of weights/beams at a known distance. The wheel includes a precision drive machined into the boss to fit a wide range of devices to be calibrated. The boss is easily interchangeable if an alternative drive size is required. The calibration wheel uses kg and g masses. Precision weight pans and counterweight set; cables; suspension hooks and a robust carry case are included. A UKAS calibration is available on request.

SPECIFICATION

- Uncertainty of Measurement better than 0.045% of reading.
- Both 1/4" Square and 1/4" Hex drive as standard for calibration of a wide range of torque measuring devices.
- Cable, hooks and precision weight pan and counterweight set included.
- Designed to be used with kg and g weights.
- Easily interchangeable boss for alternative drive sizes.
- UKAS calibration available on request.
- Precision masses available (See page 53).

DIMENSIONS

Overall Diameter: 104mm

Thickness: 10mm across boss

Length of cable: approximately 400mm per side

Advanced Witness Systems Ltd © 2024

Model:

UCB-Maximum

Torque:

Diameter:

3029

2.5Nm

104mm

MANUFACTURER INFORMATION	SUPPLIER INFORMATION
Advanced Witness Systems Ltd	
Unit 8	
Beaumont Business Centre	
Beaumont Close	
Banbury	
OX16 1TN	
Tel: +44 (0)1295 266939	
Email: sales@awstorque.co.uk	

WEIGHTS SET FOR 2NM UNSUPPORTED CALIBRATION WHEEL



Product images are for illustrative purposes only and may differ from the actual product.

DESCRIPTION

AWS can provide a set of 15 precision brass weights for calibrations up to 2Nm. A calibration certificate is included and the weights are supplied in a robust carry case. Additionally, a UKAS calibration is available on request.

SPECIFICATION

- Metric kg and g weights.
- M1 Tolerance weights set as standard.
- Other Tolerances available on request.
- Robust carry case included.
- UKAS calibration available on request.

Table of weights provided

Mass	Quantity	Mass	Quantity
1g	1	100g	1
2g	2	200g	2
5g	1	500g	1
10g	1	1kg	1
20g	2	2kg	2
50g	1		



Product images are for illustrative purposes only and may differ from the actual product.

MORE INFORMATION ON OUR PRODUCT RANGE IS AVAILABLE IN SEPARATE DATA SHEETS ON THE AWS WEBSITE WWW.AWSTORQUE.CO.UK.

Advanced Witness Systems Ltd © 2024

MANUFACTURER INFORMATION
Advanced Witness Systems Ltd
Unit 8
Beaumont Business Centre
Beaumont Close
Banbury
OX16 1TN
Tel: +44 (0)1295 266939
Email: sales@awstorque.co.uk

SUPPLIER INFORMATION

2 NM CALIBRATION MACHINE

DESCRIPTION


The AWS LTD 2Nm Calibration Machine (CR1020), designed to calibrate torque transducers, torque watches and torque screwdrivers, up to 2 Nm.

It is highly accurate and uses a disc and weights to apply torque. Weights are applied at a known distance on the circumference of the disc via balanced suspension cords and weight pans.

The Versatile 2Nm calibration machine enables the tool to be accurately positioned, and held for calibration. Adjustable levelling feet with the spirit level indication allow it to be used on a variety of bench surfaces.

SPECIFICATIONS

Capacity:	0.05 cNm to 2.0 N.m.
Uncertainty of measurement:	+/- 0.2%
Mounting:	Bench mounted with levelling indication and adjustment.
Maximum mechanical overload:	125% of Range stated.
Operating temperature:	20°C.
Directions of use:	Clockwise and anti-clockwise calibration. +/-270 degrees of rotational freedom to accommodate torque watches
Capability:	All types of torque watch, AWS IITT-1011 and third party torque transducers. It can also be used with a variety of other very small torque measuring devices.

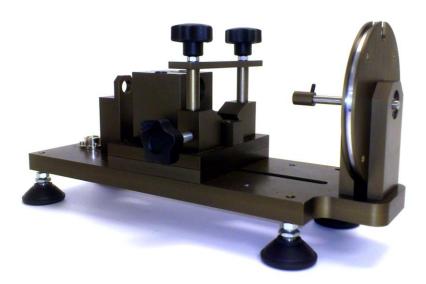

Advanced Witness Systems Ltd © 2024

MANUFACTURER INFORMATION Advanced Witness Systems Ltd

Unit 8 Beaumont Business Centre Beaumont Close Banbury OX16 1TN Tel: +44 (0)1295 266939 Email: sales@awstorque.co.uk

SUPPLIER INFORMATION

ADMS SOFTWARE

Our software arm

ADVANCED DATA & MEASUREMENT SERIES

designs and produces torque tool and torque transducer calibration, uncertainty calculation and certification software for use with PC's.

Our software can be used to improve calibration accuracy & efficiency, tracking tools & customers, and removing the need for spreadsheets.

Our Kepler 4 software is our most comprehensive torque tool calibration software on the market today, for the calibration and certification of torque wrenches to BS EN ISO 6789:2017, 2003 or your own in-house standards, and for keeping track of each individual wrench.

ADMS Software	PAGE
Kepler 4 Software Comparison	56
Kepler 4 Combined	57-58
Kepler 4 Conformity	59-60
Kepler 4 Calibration	61-62
K Factor Verification Module	63

Advanced Witness Systems Ltd Catalogue 2024 Data was correct at time of publication. Catalogue Page 55

KEPLER 4 SOFTWARE COMPARISON

				Kepler 4	
Feature	Kepler Lite 3	Kepler 3	Conformity		Combined
Complies with ISO 6789:2003 and BS EN 26789:2003 torque standards.	✓	✓	√	✓	✓
Full tracking of tool tightening performance.	✓	✓	✓	✓	✓
Full tracking of tools calibration performance and history.	✓	✓	✓	✓	 ✓
Tool performance & data input via COM port and keyboard. Option for					
bar code direct entry.	✓	✓	✓	~	~
Shows torque out of limits for selected tool.	✓	✓	✓	✓	✓
Automatically calculates average and deviation of each set of readings.	✓	✓	✓	✓	✓
User generated database for tool types and torque parameters	 Image: A set of the set of the	×	 Image: A set of the set of the	1	×
required.	•	•	•	•	•
Data output and report generation collated and filtered from any	1		1	1	1
combination of good and out of tolerance tools. Uses include monthly	~	~	~	~	~
reports, etc. Calibration Instrument/Machine/Inspection details.	✓				✓
Bespoke templates easily created for your certificates, reports and					
labels.	✓	✓	✓	 ✓ 	✓
Auto or manual certificate numbering.	✓	✓	✓	✓	✓
All certificate print details recorded. Enables exact facsimile	 ✓ 	~	 ✓ 	 Image: A second s	 ✓
reproduction.	~	*	v	v	~
Select different printers for readings, labels, and reports/certificates.	✓	✓	✓	✓	✓
Translation screens and print out can be converted to the language of	✓	v	×	×	✓
your choice.					
Multiple operator accounts (With password protection).	✓	✓	✓	✓	✓
Produce a report listing tools that require calibrating.		✓	✓	✓	✓
Tool identification and serial number identification.		✓	✓	✓	✓
Fast tool search by user set criteria.		✓	✓	✓	✓
Tool area and station location.		✓	✓	✓	✓
Cloning facility speeds multiple tool data entry.		 ✓ 	✓	✓	✓
Colour configuration.		✓	✓	✓	✓
Complies with BS EN ISO 6789:2017 Part 1, allowing the automatic			 Image: A set of the set of the		 Image: A set of the set of the
calculation of the mean deviation and mean value for each setting.			•		•
Calculates the deviation for each reading, and indicates by colour			✓		✓
whether the reading is within tolerance to the selected standard. Complies with BS EN ISO 6789:2017 Part 2, allowing the automatic					
calculation using new formulae of the mean, deviation and combined				×	1
uncertainty of each set of readings, for each torque tool.				·	
Full tracking of tools calibration performance and history. Produce a				1	1
report listing tools that require calibrating.				v	~
Production Line capabilities, for hourly or daily tool reliance				 Image: A set of the set of the	✓
performance.				-	
Calculate K Factor to meet UKAS M3003 Appendices B and C. Using module purchased seperately.				✓	✓
Model readings can be analysed to generate average bod, bint and bl					
values from 10 or more tools, to be used for future tools.			✓	✓	✓
Instrument database which allows combination of 5 instrument items,			×	 ✓ 	 ✓
such as TD/Lead/Display.			v	v	~
Standards database, including ISO 6789:2017 & 2003 pre-entered.			✓	✓	✓
Historic calibration and conformity certificates can be found from					
searching by customer and tool, by works order number, or by certificate			✓	✓	✓
number. User generated databases for customers, instruments, tools, models, &					
standards.			✓	✓	✓
Fast tool entry from model database.			✓	✓	✓
Import signatures as pictures.			· ·	· ·	· · ·
			· ·	· ·	✓ ✓
Implementation of works order tracking system.			✓ ✓	✓ ✓	▼ ✓
New simplified and improved screen layouts.					
New system using .NET framework and sequel databases.			✓	✓	✓

Advanced Witness Systems Ltd © 2024

MANUFACTURER INFORMATION Advanced Witness Systems Ltd

Unit 8 Beaumont Business Centre Beaumont Close Banbury OX16 1TN Tel: +44 (0)1295 266939 Email: sales@awstorque.co.uk

SUPPLIER INFORMATION

KEPLER 4 FOR 2017 COMBINED

The combined program for the calibration and certification of torque wrenches to BS EN ISO 6789:2017, BS EN ISO 6789:2003 or your own in-house standards, and for keeping track of each individual wrench.



Kepler 4 is built around a new works orders database, which ties together the customer, tool, model, reading & certificate.

KEY CONFORMITY FEATURES

- Complies with ISO 6789:2017 Part 1, allowing the automatic calculation of the mean deviation and mean value for each setting.
- Also calculates the deviation for each reading, and indicates by colour whether the reading is within tolerance to the selected standard.

Key Calibration Features

- Complies with ISO 6789:2017 Part 2, allowing the automatic calculation using new formulae of the mean, deviation & combined uncertainty of each set of readings, for each torque tool.
- Calibrates both square and hexagonal drive wrenches.
- Full tracking of tools calibration performance and history. Produce a report listing tools that require calibrating.
- The ability to calculate average values of uncertainties Bod, Bint and BI over the last 10 calibrated tools of the same model.
- The ability to Colour the Calibration, to apply colour indicators to the results to show whether the deviation is within tolerance for the tool type as defined in ISO 6789:2017 Part 1. This can also be displayed on printed reports.

KEY SHARED FEATURES INCLUDE

- Powerful search function allows historic calibration and conformity certificates to be easily found from searching by customer, tool or model; works order number or certificate number.
- Bespoke templates easily created for certificates, reports and labels. Auto or manual certificate numbering.
- Option to operate in 6789:2003 to allow phased migration to 6789:2017.
- Tool performance & data input via COM port and keyboard. Option for bar code direct entry.
- A Miscellaneous Tools feature, allowing storage of non-torque tool information for use in recording the calibration of Miscellaneous Tools, generating overdue tool reports, and certificate front pages.
- Exporting of results data as a csv file for use in other programs.
 Advanced Data & Measurement Systems is a Trading

Advanced Data & Measurement Systems is a Trading name owned by Advanced Witness Systems Ltd © 2024 Data was correct at time of publication. Catalogue Page 57

OTHER FEATURES INCLUDE

• All certificate print details recorded. Enables exact reproduction ensuring full traceability.

Read

- Cloning facility speeds multiple data entry.
- Import and Export reports into text or spreadsheet formats for more efficient database backup.
- Databases can be converted from Kepler 3, 2002 and 2000 allowing faster start up for previous customers.
- Databases can be stored locally or on a server for more efficient backup.
- Multiple translations available, including the facility to create your own translation.
- Data output and report generation collated and filtered from any combination of good and out of tolerance tools.
- Comprehensive user manual.
- Free demonstration and 6 months full help and support included in purchase.
- Certificate conversion available on enquiry.
- **NEW!** K factor verification to UKAS M3003 Appendices B and C using external spreadsheet module (Sold Separately).

SYSTEM REQUIREMENTS:

Minimum Screen Resolution: 1280x768.

Software is a .NET application using an SQL Database.

Minimum System: i5 Processor or equivalent, 4GB RAM, on board graphics. Keyboard & Mouse Interface.

Disclaimer: This datasheet may not reflect the latest version of the software. For more information, visit our website: www.awstorque.co.uk.

ALSO AVAILABLE AS SEPARATE CONFORMITY	AND CALIBRATION VERSIONS
Advanced Data & Measurement Syste Advanced Witness Sy	v
MANUFACTURER INFORMATION Advanced Witness Systems Ltd Unit 8 Beaumont Business Centre Beaumont Close Banbury OX16 1TN Tel: +44 (0)1295 266939 Email: sales@awstorque.co.uk	SUPPLIER INFORMATION
Data was correct at tim Catalogue Pa	

Readings	readings				wint Readings		wl Readings		
Readings:								Reading Co	ontrol:
Regul	lar Readings	_	ominal Torque:		n				
	Setting 1	Setting 2		ting 3				Sa	ve and Continue
Setting	: 10.000 N.m	30.000 N.m	50.00	10 N.m					
								Cles	ar These Readings
Reading 1	10.000	30.00	00	50.000				Re	view All Readings
Reading 2	10.000			50.000					
Reading 3	t: 10.000			50.000				Re	istart All Readings
Reading 4	10.000	30.00	0	50.000					
Deading 5	10.000	30.00	00	50.000					
Kepled Control	New Works Order								ting Setings
								Repor	nng Settings
Current Works Ord Works Order Det		Brows	e Works Orders		Selected Cus Cust	omer ID: CU	ST1		Check Custome
Works Order 1	No: X000500/03		All Works Orders		Customer 1				-
	Check Works 0	Inder	Unassigned		View Custor	mer List	All Customers	Edit Custon	ner New Customer
CUST1 - Custome			Selected Custor						
TODL1 - Testing 1			elected Custome			Tool ID: TO	OL1		Check Tool
Readings Comple	ebe		Order Action:		Testing Tool				
18/01/2018 09:02:2	425-31-838-1				View Too	J I	ist All Tools	Edit Too	I New Tool
Calibration Rea	iding		idate Customer/T					Custome	r/Tool Action:
			ld Reading Det						View All Readings
Calibration	SelectCus	4Tool	View Works Orde						
								35	ave Page Defaults
International Action	A Anialan and	10 1		Sector Contractor	UKALI AL AL		-	Constant	vanced Witness Systems 2
inter Aurin Operato	r (reachinestrator)	to January 2018 10		Neplett - Versio	enter 101 - Calibri	asch and Conk	annay	copyignte: Ad	vances wimess systems 2
Colibratic - Incl	ment and Lab Settin								
	ment and Lab Settin	ngs.							
in the second				beatwood .					
2206	Description 10Nm ITT		Select>>	Instrument	Descriptio	on		Combined expa device unce	nded measuring ertainty (Wmd %) 0.0
2206 2356	Description 10Nm ITT 50Nm ITT		Select>>	Instrument	Descriptio	n		device unce	ertainty (Wmd %)
2206 2356 2460	Description 10Nm ITT 50Nm ITT ITT - 1013 - 50Nm		Select>>	Instrument	Descriptio	n		device unce	ended measuring entainty (Wmd %) teasuring device ent error (bep %)
2205 2356 2460 2492 2812	Description 10Nm IITT 50Nm IITT IITT - 1013 - 50Nm 250Nm IITT 500Nm IITT		Select>>	Instrument	Descriptio	n		device unce	ertainty (Wmd %)
2205 2356 2460 2492 2812	Description 10%mITT 50Nm IITT IITT - 1013 - 50Nm 250Nm IITT		< Deselect		Descriptio	on		device unce Selected m measurem	entainty (Wmd %) 00 reasuring device ent error (bep %) 0.0
2205 2356 2460 2492 2812 2935	Description 10Nm IITT 50Nm IITT IITT - 1013 - 50Nm 250Nm IITT 500Nm IITT		Select>>	rre 'C: 20		n		device unce Selected m measurem nidity %: 40	ertainty (Wmd %) 00 teasuring device ent error (bep %) 00
2205 2356 2460 2492 2812 2935 Standard Setup:	Description 10Nm ITT 50Nm ITT ITT - 1013 - 50Nm ITT - 1013 - 50Nm ITT 500Nm ITT 1500Nm ITT		<deselect Lab Temperatu</deselect 	re 'C: 20 Readi	ng Settings:		Lab Hur	device unce Selected m measurem nidity %: 40	entainty (Wmd %) 00 reasuring device ent error (bep %) 0.0
2205 2356 2460 2492 2812 2935 Standard Setup:	Description 10Nm IITT 50Nm IITT IITT - 1013 - 50Nm 250Nm IITT 500Nm IITT		<deselect Lab Temperatu</deselect 	re 'C: 20 Readi				device unce Selected m measurem nidity %: 40 Use Defax bod (Va	etainty (Wmd %) 00 neasuring device ent error (bep %) 00 alt Model Values: riation due to cutput drive.
2205 2256 2460 2492 2812 2935 5tandard Setup: 6789:2017	Description 10%m IIT 50Nm IIT UTT - 1013 - 50Nm UTT - 1013 - 50Nm UTT - 1013 - 50Nm UTT - 1013 - 50Nm UTT - 1013 - 50Nm 0 6789-2003		<deselect Lab Temperatu</deselect 	re 'C: 20 Readi	ng Settings: ominal Torque:	50.0	Lab Hur	device unce Selected m measurem nidity %: 40 Use Defas bod (Va bint (Var	etainty (Wmd %) 000 eeasuning device ent emor (bep %) 000 alt Model Values: ristion due to output drive; ristion due to interface)
2206 2256 2460 2492 2812 2935 Standard Setup: 0 67892017 Standard (20/76/2017/11)	Description 10%m1TT 50%m1TT 50%m1TT 117 - 1013 - 50Nm 250%m11TT 500%m1TT 1500%m1TT 0 6789.2003 Description TIGA Weekh tone	In-House	<deselect lab="" standard<="" td="" temperatu=""><td>re 'C: 20 Readi</td><td>ng Settings: ominal Torque: Setting 1:</td><td>50.0</td><td>Lab Hur</td><td>device unce Selected m measurem midity %: 40 Use Defas bod (Va bint (Var bint (Var bint (Var</td><td>etainty (Wmd %) 000 eeasuting device ent error (bep %) 000 att Model Values: ination due to interface) Ioading point variation)</td></deselect>	re 'C: 20 Readi	ng Settings: ominal Torque: Setting 1:	50.0	Lab Hur	device unce Selected m measurem midity %: 40 Use Defas bod (Va bint (Var bint (Var bint (Var	etainty (Wmd %) 000 eeasuting device ent error (bep %) 000 att Model Values: ination due to interface) Ioading point variation)
2206 2256 2460 2492 2812 2935 3tandard Setup: 0 6789:2017 Standard	Description 10%m1TT 50%m1TT ITT-1013-50Nm 250%m1TT 350Nm1TT 1500Nm1TT 0 6789-2003 Description 11GX Wreach, torst	In-House	<deselect dial="" display<="" lab="" or="" standard="" td="" temperatu=""><td>re 'C: 20 Readi</td><td>ng Settings: orminal Torque: Setting 1: Setting 2:</td><td>50.0 20% ** 60%</td><td>Lab Har 0 N·m 10.00 30.00</td><td>device unce Selected m measurem nidity %: 40 Use Defax bod (Va bint (Var bint (Var bint (Var</td><td>etainty (Wmd %) 000 easeming device ent error (bep %) 000 alt Model Values: ration due to output divise (addon due to interface) loading point variation) ve Selection (wod):</td></deselect>	re 'C: 20 Readi	ng Settings: orminal Torque: Setting 1: Setting 2:	50.0 20% ** 60%	Lab Har 0 N·m 10.00 30.00	device unce Selected m measurem nidity %: 40 Use Defax bod (Va bint (Var bint (Var bint (Var	etainty (Wmd %) 000 easeming device ent error (bep %) 000 alt Model Values: ration due to output divise (addon due to interface) loading point variation) ve Selection (wod):
2205 2356 2460 2492 2812 2935 Standard Setup: 6789:2017 Standard 506789:2017-T1. 506789:2017-T1. 506789:2017-T1.	Description 10%m1TT 50%m1TT IIT-1013-50%m 250%m1TT 350%m1TT 1500%m1TT 1500%m1TT 1500%m1TT 150%meek, npd 11CB: Vireach, npd 11CB: Vireach, npd 11CD: Screedinger, 11CD: Scree	In House In or ferrior bar housing with scale, of housing and electro	< Deselect >> Lab Temperature Standard Sial or display nic measurem play	re 'C: 20 Readi	ng Settings: ominal Torque: Setting 1:	50.0 20%** 60% 100%	Lab Har 0 N m 10.00 30.00 50.00	device unce Selected m measurem nidity %: 40 Use Defax bod (Va bint (Var bint (Var bint (Var	etainty (Wmd %) 000 easuring device ent error (bep %) 000 alt Model Values: ration due to interface) a loading point variation) ve Selection (wod-0)
2205 2356 2460 2492 2812 2935 36andard Setap: 367892017 Standard 506789201711 506789201711 506789201711	Description 10km11T 50Nm11T 50Nm11T 50Nm11T 50Nm11T 500Nm11T 1500Nm11T	In-House on of feace bar housing with scale, c housing with scale, c housing with scale, c	< Deselect Lab Temperatur Standard fial or display nic measurem play rement	re 'C: 20 Readi	ng Settings: orminal Torque: Setting 1: Setting 2:	50.0 20%** 60% 100%	Lab Har 0 N·m 10.00 30.00	device unce Selected m measurem midty %: 40 Use Defas bot (Va bit (Va bit (Va bit (Va Output Drite 0 4 Positic Interface S	entainty (Wmd %) 05 executing devices enter (thep %) 05 eff (Model Values: instand due to extpand diver labon due to extpand diver labon due to restrates) labon due to restrates) escandar port variants labon due to restrates) escandar port variants of the second selection (wint):
2205 2356 2460 2492 2492 2935 Standard Setup: 0 6789.2017 Standard Stor789.2017-11. Stor789.2017-11. Stor789.2017-11. Stor789.2017-11. Stor789.2017-11. Stor789.2017-11. Stor789.2017-12. Stor789.2017-13. Stor789.	Description 10km 11T 50Nm 11T 10T-1013-50Nm 11T-1013-50Nm 11T 500Nm IIT 500Nm IIT 150N Wrech boso 11Cb Kreech, njd 11Cb Kreech,	In House In House housing with scale, of housing, and electron with scale, dial or dis with electronic measu with electronic measu	< Deselect Ceselect Lab Temperatu Standard dal or display nicimeasurem play rement did displayer	re 'C: 20 Readi	ng Settings: orminal Torque: Setting 1: Setting 2:	50.0 20% ** 60% 100% Rec	Lab Har 0 N m 10.00 30.00 50.00	device unco Selected m measurem midty %: 40 Use Defae b of (Var b to (Var D to (Var Output Dri Tool has 0 4 Positic Interface \$ 0 No aday	etainty (Wmd %) 005 etainty (Wmd %) 005 etainty (bap %) 005 etainty (bap %) 005 etainty (bap %) etainty (bap %
2005 2036 2460 2492 2812 2935 3tandard Setup: 9 67892017 506789201771 506789201771 506789201715 506789201712 506789201712	Description 10km 11T 50Nm 11T 10T-1013-50Nm 11T-1013-50Nm 11T 500Nm 11T 500Nm 11T 1500Nm 11T	In House on of feation bat housing with scale, of housing, and electron with scale, dial or dis with electronic massas with electronic massas with electronic massas with electronic massas ababe, snortunated or w ladjustment stable, morganshalle	< Deselect Lab Temperatu Standard	re 'C: 20 Readi	ng Settings: orminal Torque: Setting 1: Setting 2:	50.0 20%** 60% 100% Rec	Lab Hur 0 N m 10.00 50.00 alculate • Clockwise	device unice Selected m measurem midly %: 40 Use Defas Dod (Va Def (Var Def (Var Def (Var Def (Var Def (Var Def (Var Def (Var Def (Var) Def	entainty (Wmd %) 05 entainty (Wmd %) 05 ent ener (bep %) 05 ent Model Values: intition due to interface) isoland port interface isoland port isoland isoland isoland iso
2005 2036 2460 2492 2812 2935 3tandard Setup: 9 67892017 506789201771 506789201771 506789201715 506789201712 506789201712	Description 10km 11T 50Nm 11T 10T-1013-50Nm 11T-1013-50Nm 11T 500Nm IIT 500Nm IIT 150N Wrech boso 11Cb Kreech, njd 11Cb Kreech,	In House on of feation bat housing with scale, of housing, and electron with scale, dial or dis with electronic massas with electronic massas with electronic massas with electronic massas ababe, snortunated or w ladjustment stable, morganshalle	< Deselect Lab Temperatu Standard	re °C: 20 Readi N	ng Settings: ominal Torque: Setting 1: Setting 2: Setting 3:	50.0 20%** 60% 100% Rec	Lab Hur 0 N m 10.00 30.00 50.00 alculate	device unice Selected m measurem Midley %: 40 Use Defae b d (Va b d (Va) d (Va b d (Va) d (V	etainty (Wmd %) 005 etainty (Wmd %) 005 etainty (bap %) 005 etainty (bap %) 005 etainty (bap %) etainty (bap %
2255 2266 2460 2482 2832 2835 2835 2835 2835 2835 2835 28	Description 10km 11T 50Nm 11T 10T-1013-50Nm 11T-1013-50Nm 11T 500Nm 11T 500Nm 11T 1500Nm 11T	In House on or flancon bar housing, and selectro with scale, dial or disp with electroic measu stable, oraginatured or adjusther, graduated adjusther, graduated adjusther, graduated	< Deselect Lab Temperatur Standard	re °C: 20 Readi N	ng Settings: orminal Torque: Setting 1: Setting 2:	50.0 20%** 60% 100% Rec	Lab Hur 0 N m 10.00 50.00 alculate • Clockwise	device unice Selected m measurem nidly %: 40 Use Defas bit (Vas bit (Vas bi	entainty (Wmd %) 08 wasseling devices ent energ (bep %) 08 wasseling devices ent energ (bep %) 08 wasseling between the source of the source o
2205 2266 2460 2482 2832 2835 2835 29 26782017 20 27 20 27 20 27 20 27 20 27 20 27 20 27 20 20 20 20 20 20 20 20 20 20 20 20 20	Description 10km 11T 50Nm 11T 10T-1013-50Nm 11T-1013-50Nm 11T 500Nm 11T 500Nm 11T 1500Nm 11T	In House on or flancon bar housing, and selectro with scale, dial or disp with electroic measu stable, oraginatured or adjusther, graduated adjusther, graduated adjusther, graduated	< Deselect Lab Temperatur Standard	re °C: 20 Readi N	ng Settings: ominal Torque: Setting 1: Setting 2: Setting 3:	50.0 20%** 60% 100% Rec	Lab Hur 0 N m 10.00 50.00 alculate • Clockwise	device unice Selected m measurem nicity %: 40 Use Defas bit (Vas bit (Vas b	entainty (Wimd %) 0.00 entainty (Wimd %) 0.00 ent enters (bep %) 0.00 ent enters (bep %) 0.00 ent to bishoftical ent block Values: initiation due to captio divert initiation due to captio divert initiation due to captio divert enters (beginstream) 0.00 enters (beginstream) 0.00 e
2205 2266 2460 2482 2832 2835 2835 29 267692017 20 27 267692017 20 27 27 20 27 27 27 27 27 27 27 27 27 27 27 27 27	Description 10km 11T 50Nm 11T 10T-1013-50Nm 11T-1013-50Nm 11T 500Nm 11T 500Nm 11T 1500Nm 11T	In House on or flancon bar housing, and selectro with scale, dial or disp with electroic measu stable, oraginatured or adjusther, graduated adjusther, graduated adjusther, graduated	< Deselect Lab Temperatur Standard	re °C: 20 Readi N	ng Settings: ominal Torque: Setting 1: Setting 2: Setting 3:	50.0 20% ** 60% 100% Rec valion)	Lab Hur 0 N m 10.00 30.00 30.00 30.00 30.00 30.00 20.0	device unice Selected m measurem midly %: 40 Use Defax beit (Var beit (Var t (Force Output Dri O 4 Positis Interface S O 4 Positis Force Loa O 4 Positis	estavity (Wmd %) 000 estavity (Wmd %) 000 estaves develop %) 000 estaves develop %) 000 estaves develop %) estaves develop % estaves develop % estaves develop estaves d
2205 2266 2460 2482 2832 2835 2835 29 267692017 20 27 267692017 20 27 27 20 27 27 27 27 27 27 27 27 27 27 27 27 27	Description 10km 11T 50Nm 11T 10T-1013-50Nm 11T-1013-50Nm 11T 500Nm 11T 500Nm 11T 1500Nm 11T	In House on or flancon bar housing, and selectro with scale, dial or disp with electroic measu stable, oraginatured or adjusther, graduated adjusther, graduated adjusther, graduated	< Deselect Lab Temperatur Standard	re °C: 20 Readi N	ng Settings: ominal Torque: Setting 2: Setting 3: west scale grade	50.0 20% ** 60% 100% Rec vation)	Lab Har 10.00 30.00 50.00 alculate Clockwise Counter Clock	device unice Selected m measurem midly %: 40 Use Defax beit (Var beit (Var t (Force Output Dri O 4 Positis Interface S O 4 Positis Force Loa O 4 Positis	entainty (Wimd %) 0.00 entainty (Wimd %) 0.00 ent enters (bep %) 0.00 ent enters (bep %) 0.00 ent to bishoftical ent block Values: initiation due to captio divert initiation due to captio divert initiation due to captio divert enters (beginstream) 0.00 enters (beginstream) 0.00 e
2205 2266 2460 2482 2832 2835 2835 29 267692017 20 27 267692017 20 27 27 20 27 27 27 27 27 27 27 27 27 27 27 27 27	Description 10km 11T 50Nm 11T 10T-1013-50Nm 11T-1013-50Nm 11T 500Nm 11T 500Nm 11T 1500Nm 11T	In House on or flancon bar housing, and selectro with scale, dial or disp with electroic measu stable, oraginatured or adjusther, graduated adjusther, graduated adjusther, graduated	< Deselect Lab Temperatur Standard	re °C: 20 Readi N	ng Settings: ominal Torque: Setting 1: Setting 2: Setting 3:	50.0 20% *** 60% 100% Rec vation)	Lab Har 10.00 30.00 50.00 alculate Clockwise Counter Clock	device unice Selected m measurem midty %: 40 Use Defais o do (% Def (Force Output Dff) Tool har O No aday O No aday O No App Force Loa No App	Heating (Wind TG) 42 (42) Heating (Wind TG) 42
2005 2366 2460 2492 2812 2935 Standard Setup: 0 6789:2017 Standard 0 (20: 20: 20: 20: 20: 20: 20: 20: 20: 20:	Description 10km 11T 50Nm 11T 10T-1013-50Nm 11T-1013-50Nm 11T 500Nm 11T 500Nm 11T 1500Nm 11T	In House on or flancon bar housing, and selectro with scale, dial or disp with electroic measu stable, oraginatured or adjusther, graduated adjusther, graduated adjusther, graduated	 Standard Standard<	re °C: 20 Readi N	ng Settings: ominal Torque: Setting 2: Setting 3: west scale grade	50.0 20% ** 60% 100% Rec vation)	Lab Har 10.00 30.00 50.00 alculate Clockwise Counter Clock	device unice Selected m measurem midty %: 40 Use Defais o do (% Def (Force Output Dff) Tool har O No aday O No aday O No App Force Loa No App	estavity (Wmd %) 000 estavity (Wmd %) 000 estaves develop %) 000 estaves develop %) 000 estaves develop %) estaves develop % estaves develop % estaves develop estaves d
2205 2266 2460 2482 2832 2835 2835 29 267692017 20 27 267692017 20 27 27 20 27 27 27 27 27 27 27 27 27 27 27 27 27	Description 10km 11T 50Nm 11T 10T-1013-50Nm 11T-1013-50Nm 11T 500Nm 11T 500Nm 11T 1500Nm 11T	In House on or flancon bar housing, and selectro with scale, dial or disp with electroic measu stable, oraginatured or adjusther, graduated adjusther, graduated adjusther, graduated	< Deselect Lab Temperatur Standard	re °C: 20 Readi N	ng Settings: ominal Torque: Setting 2: Setting 3: west scale grade	50.0 20% ** 60% 100% Rec vation)	Lab Har 10.00 30.00 50.00 alculate Clockwise Counter Clock	device unice Selected m measurem midty %: 40 Use Defais o do (% Def (Force Output Dff) Tool har O No aday O No aday O No App Force Loa No App	Heating (Wind TG) 42 (42) Heating (Wind TG) 42
2006 2006 2006 2006 2007 2007 2007 2007	Description Version 117 Softwart 117 Soft	In House on or flancon bar housing, and selectro with scale, dial or disp with electroic measu stable, oraginatured or adjusther, graduated adjusther, graduated adjusther, graduated	Satisfield >> < Deselect Lab Temperatu Standard Standard di or display nic measurem play rement ath display d or with displa or with displa cotion: Statistic (179-201) adding (1-9) Satisfield (1-9) catulated (1-9) catul	re °C: 20 Readi N (** or lo 7 isse Readings. wise africans. atoms.	ng Settings: ominal Torque: Setting 2: Setting 3: west scale grade	50.0 20% ** 60% 100% Rec vation)	Lab Har 10.00 30.00 50.00 alculate Clockwise Counter Clock	device unic Selected m measurem nicity %: 40 Use Defae 0 60 (Vs 0	entenny (Mini ST) 48 44 enseming diversified and an enseming diversified and and Model Values: entend due to a subject field and diversified and an enseming to a diversified and an enseming to a diversified and an enseming we called a diversified and and and and diversified and an enseming we called and and an enseming the standard and an enseming the standard and and and and and and and an enseming the standard and and and and and and an enseming the standard and
2205 2266 2460 2482 2832 2835 2835 29 267692017 20 27 267692017 20 27 27 20 27 27 27 27 27 27 27 27 27 27 27 27 27	Description Softwart FT Softwart FT Softw	In House	< Deselect Lab Temperatur Standard	re °C: 20 Readi N (** or lo 7 isse Readings. wise africans. atoms.	ng Settings: ominal Torque: Setting 2: Setting 3: west scale grade	50.0 20% ** 60% 100% Rec vation)	Lab Har 10.00 30.00 50.00 alculate Clockwise Counter Clock	device unice Selected m measurem midty %: 40 Use Defais o do (% bit (%arc Output Dir) O Tool har O No aday O No aday O No aday O No App Force Loa No App	entering (Wine ST) = 81 est entering (Wine ST) = 82 est entering the scale of the
2006 2366 2460 2460 2595 2595 2595 2595 2595 2595 2595 259	Description Description Solven ITT Solven ITT Solven ITT Solven ITT Solven ITT Solven ITT Solven ITT Solven ITT CC Stream Const TCC Watch fug TCC Watch fug TC	In the second seco	Statuct 1>> Cheeselect Lab Temperature Standard <p< td=""><td>re 'C: 20 Readin N /* or lo 7 see Readings. mice alicons. alicons.</td><td>setting: setting: Setting: Setting: Setting: Setting: Setting: Setting: Setting: TrcA F</td><td>50.00 20% ** 60% 100% Rec 0 0 0 0 0 0</td><td>Lab Har 10.00 30.00 50.00 alculate Clockwise Counter Clock</td><td>device unic Selected m measurem nicity %: 40 Use Defae 0 60 (Vs 0 60 (Vs 0</td><td>A Nodel Value: an A Nodel Value: A Nodel Val</td></p<>	re 'C: 20 Readin N /* or lo 7 see Readings. mice alicons. alicons.	setting: setting: Setting: Setting: Setting: Setting: Setting: Setting: Setting: TrcA F	50.00 20% ** 60% 100% Rec 0 0 0 0 0 0	Lab Har 10.00 30.00 50.00 alculate Clockwise Counter Clock	device unic Selected m measurem nicity %: 40 Use Defae 0 60 (Vs 0	A Nodel Value: an A Nodel Value: A Nodel Val
2006 2006 2006 2007 2007 2007 2007 2007	Description Description Solven ITT Solven ITT Solven ITT Solven ITT Solven ITT Solven ITT Solven ITT Solven ITT CC Stream Const TCC Watch fug TCC Watch fug TC	In the second seco	Statuct 1>> Cheeselect Lab Temperature Standard <p< td=""><td>re 'C: 20 Readin N /* or lo 7 see Readings. mice alicons. alicons.</td><td>ng Settings: ominal Torque: Setting 2: Setting 3: west scale grade</td><td>50.00 20% ** 60% 100% Rec 0 0 0 0 0 0</td><td>Lab Har 10.00 30.00 50.00 alculate Clockwise Counter Clock</td><td>device unic Selected m measurem nicity %: 40 Use Defae 0 60 (Vs 0 60 (Vs 0</td><td>entenny (Mini ST) 48 44 enseming diversified and an enseming diversified and and Model Values: entend due to a subject field and diversified and an enseming to a diversified and an enseming to a diversified and an enseming we called a diversified and and and and diversified and an enseming we called and and an enseming the standard and an enseming the standard and and and and and and and an enseming the standard and and and and and and an enseming the standard and</td></p<>	re 'C: 20 Readin N /* or lo 7 see Readings. mice alicons. alicons.	ng Settings: ominal Torque: Setting 2: Setting 3: west scale grade	50.00 20% ** 60% 100% Rec 0 0 0 0 0 0	Lab Har 10.00 30.00 50.00 alculate Clockwise Counter Clock	device unic Selected m measurem nicity %: 40 Use Defae 0 60 (Vs 0	entenny (Mini ST) 48 44 enseming diversified and an enseming diversified and and Model Values: entend due to a subject field and diversified and an enseming to a diversified and an enseming to a diversified and an enseming we called a diversified and and and and diversified and an enseming we called and and an enseming the standard and an enseming the standard and and and and and and and an enseming the standard and and and and and and an enseming the standard and
2006 2006 2006 2007 2007 2007 2007 2007	Description Description Solow IIT Solow I	In the second seco	Statuct 1>> Cheeselect Lab Temperature Standard <p< td=""><td>ve °C 20 Reading N N N N N N N N N N N N N N N N N N N</td><td>setting: setting: Setting: Setting: Setting: Setting: Setting: Setting: Setting: TrcA F</td><td>50.00 20%** 60% 100% Rec 0 (0 0 0 0 0 0 0 0 0 0 0 0 0</td><td>Lab Har 10.00 30.00 50.00 alculate Clockwise Counter Clock</td><td>device unice Siellected m medstures and the second of the second of the second of the second of the second of the second of the</td><td>status (minist) 21 22 23 23 23 23 23 23</td></p<>	ve °C 20 Reading N N N N N N N N N N N N N N N N N N N	setting: setting: Setting: Setting: Setting: Setting: Setting: Setting: Setting: TrcA F	50.00 20%** 60% 100% Rec 0 (0 0 0 0 0 0 0 0 0 0 0 0 0	Lab Har 10.00 30.00 50.00 alculate Clockwise Counter Clock	device unice Siellected m medstures and the second of the second of the second of the second of the second of the second of the	status (minist) 21 22 23 23 23 23 23 23
2006 2016 2016 2016 2017 2017 2017 2017 2017 2017 2017 2017	Description Generations Gener	Cathorner:	Seectory (Despective) Standard Stand	ve °C 20 Reading N N N N N N N N N N N N N N N N N N N	ng Settings: ominal Torque: Seting 1: Seting 2: Seting 3: TTCA: TTCA: TTCA: TTCA: TTCA: Seting 1: Calculator	50.00 20%** 60% 100% Rec 0 (0 0 0 0 0 0 0 0 0 0 0 0 0	Lab Har DNm 1000 100	device unic Sieliceto d'im- medature midity %: 40 Use Datas 0 of 0 40 0 of 0 0 0 of 0 0 0 of 0 0 0 of 0 of 0 0 0 of 0 of 0 0 0 of 0 0 0 of 0 of 0 0 0 of 0 0	estating (Wine STG) e
2006 2006 2006 2007 2007 2007 2007 2007	Description Generations Gener	Control of the second	Search	ve °C 20 Reading N N N N N N N N N N N N N N N N N N N	seting 2 Seting 2 Seting 3 Seting 2 Seting 3 TCA E C Seting 3 TCA E Seting 3 Seting 4 Seting	50.00 20%** 60% 100% Rec 0 (0 0 0 0 0 0 0 0 0 0 0 0 0	Lab Har Nm 1600 3000 500 5000 5	device unic Sieliceto d'im- medature midity %: 40 Use Datas 0 of 0 40 0 of 0 0 0 of 0 0 0 of 0 0 0 of 0 of 0 0 0 of 0 of 0 0 0 of 0 0 0 of 0 of 0 0 0 of 0 0	search (Wind T) = 0 = 0 = 0 = 0 = 0 = 0 = 0 = 0 = 0 =
2006 2016 2016 2016 2017 2017 2017 2017 2017 2017 2017 2017	Desception Desception Sideward T Sideward T Sideward T Sideward T Sideward T Sideward T Sideward T Sideward T Colores T C	Catherine Cathe	Search 2 Cluster Lab Temperature Standard did or dopty did or dopty did or or the digital did or or the digital did or or the digital did or or the digital cluster Cluster Cluster Cluster Terroris Standard State Search 2 Search 2 Sea	ve °C 20 N N Pecadit N N Parado N N N N N N N N N N N N N N N N N N N	g Setting: const Foreign const Fore	50.00 20%************************************	Lab Har SNM 100 1000 1000 1000 1000 1000 1000 100	derice wird Selection B medal etc. medal etc. Meda	estanty (Wine TG)
2006 2016 2016 2016 2017 2017 2017 2017 2017 2017 2017 2017	Desception Desception Sideward TT - 1017 Kills Sideward TT - 1017 Kills Sideward TT - 1017 Kills Sideward Sideward Sideward Sideward Sideward Sideward Sideward Sideward Construction Sideward Sideward Sideward TCC Wreach rule Sideward Sideward Sideward Sideward TCC Wreach rule Sideward Sidew	Control of the second	search	ve C 20 Peada N Particle Peada N Peada N Particle Peada N	state sets	50 00 20% ** 50% 10% Rec 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0	Lab Har 0 Nm 10 00 3000 3000 3000 Souther Cock Participant Souther Cock Participant Partici	derice uncertain derice uncertain derice uncertain der derice uncertain der derice uncertain der	search (Wind T) = 0 = 0 = 0 = 0 = 0 = 0 = 0 = 0 = 0 =
2006 2007	Desception Desception Sideward TT - 1017 Kills Sideward TT - 1017 Kills Sideward TT - 1017 Kills Sideward Sideward Sideward Sideward Sideward Sideward Sideward Sideward Construction Sideward Sideward Sideward TCC Wreach rule Sideward Sideward Sideward Sideward TCC Wreach rule Sideward Sidew	Catherine Cathe	Search 2 Cluster Lab Temperature Standard did or dopty did or dopty did or or the digital did or or the digital did or or the digital did or or the digital cluster Search 2 Calculated Search 2 Search 2 Se	ve °C 20 N N Pecadit N N Parado N N N N N N N N N N N N N N N N N N N	g Setting: const Foreign const Fore	50.00 20%************************************	Lab Har SNM 100 1000 1000 1000 1000 1000 1000 100	derice wird Selection B medal etc. medal etc. Meda	estanty (Wine TG)
2006 2016 2016 2016 2017 2017 2017 2017 2017 2017 2017 2017	Desception Desception Sideward TT - 1017 Kills Sideward TT - 1017 Kills Sideward TT - 1017 Kills Sideward Sideward Sideward Sideward Compared Sideward Sideward Sideward Compared Sideward Sideward Sideward Compared Sideward Sideward Sideward Sideward Compared Sideward Sideward Sideward Sideward Compared Sideward Side	Catherine Cathe	Sanctory Consoler Lab Temperature Standard dor or display pr	ve C 20 Peace Peac	series	500 20%*** 50% 100% 100% 100% 100%	Lab Har I Com 1000 10	derike wir: Switcher der wisspreicher wisspreicher Switcher der Switcher der Switcher Switcher der Switcher der Switche	estanty (Wine TG)
2006 2007	Desception Solven IT Solven IT Solven IT Solven IT Solven IT ISO0-INT Solven IT ISO0-INT TOCK Wreach, region TCCC Wreach, region TCCC Wreach, region TCCC Wreach, region TCCC Socreadings TCCC Wreach, region TCCC Wreach, region TCCC Socreadings TCCC Wreach, region	Catherine Cathe	Search 29 Chesseld Lab Temperature Lab Tempera	ve C 20 Peads N N Ye rol 2 Peads N N N N N N N N N N N N N N N N N N N	ng Setting: consul Toque Seting 2 Seting 2 Seting 2 Seting 2 Tox get to 2 Seting 2 Tox get to 2 Seting	50 00 20% ** 50% 10% Rec 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0	Lab Har 1000 100	derike wirt wirt Switcher Der medanter medanter medanter Der Deten Der	estanty (Wine TG)
2006 2007 2007 2007 2007 2007 2007 2007	Desception Desception Softwart FT Softwart FT Softwart FT Softwart FT Softwart FT Softwart FT Too Perform C Softwart FT Too Perform Softwart FT Too Perform Softwart FT Too Perform Softwart FT	Catherine Cathe	Sanctory Consoler Lab Temperature Standard dor or display pr	ve C 20 Peace Peac	series	500 20%*** 50% 100% 100% 100% 100%	Lab Har I Com 1000 10	derike wir: Switcher der wisspreicher wisspreicher Switcher der Switcher der Switcher Switcher der Switcher der Switche	estanty (Wine TG)
2006 2006 2006 2007	Desception Desception Softwart FT Softwart FT Softwart FT Softwart FT Softwart FT Softwart FT Too Perform C Softwart FT Too Perform Softwart FT Too Perform Softwart FT Too Perform Softwart FT	Catherine Cathe	Sanctory Consoler Lab Temperature Standard dor or display pr	ve C 20 Peace Peac	series	500 20%*** 50% 100% 100% 100% 100%	Lab Har I Com 1000 10	derike wir: Switcher der wegstreine wegstreine songerte Berleine B	extention (Virtual TC) extension (Virtu
2006 2007 2007 2007 2007 2007 2007 2007	Description Description Description To OT To	Catherine Cathe	Sanctory Consoler Lab Temperature Standard dor or display pr	ve C 20 Peace Peac	series	500 20%*** 50% 100% 100% 100% 100%	Labhar Labhar Son	derike wir: Switcher der wegstreine wegstreine songerte Berleine B	testany (Wine 15)
2006 2006 2006 2006 2007	Description Description Description To OT To	Control of the second	Sanctory Consoler Lab Temperature Standard dor or display pr	ve °C 20 Reading /** or lo prior Contraction statements state	series	90.0 20%-11 00% 100% Rec 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0	Lab Har I Com 1000 10	derice unit with the second se	Heating (Wine 15) Bassering General Control (Wine 15) All Model Values: All Model Va
2006 2246 2246 2246 2246 2246 2246 2246	Desception Solven IT2 Solven IT3 Solven IT3 Solven IT3 Solven IT1 So	Control of the second s	Search 2	ve C 20 Peace Peac	In the second se	500 20%*** 50% 100% 100% 100% 100%	Labhar Labhar Son	derike wir: Switcher der wegstreine wegstreine songerte Berleine B	testany (Wine 15)

KEPLER 4 FOR CONFORMITY

The program for the certification of torque wrenches to BS EN ISO 6789:2017 Part 1, BS EN ISO 6789:2003, or your own in-house standards, and for keeping track of each individual wrench.



Exit

List All Tools Edit T

Save Page Defaults

Kepler 4 is built around a new works orders database, which ties together the customer, tool, model, reading & certificate.

KEY FEATURES INCLUDE

 Complies with BS EN ISO 6789:2017 Part 1, allowing the automatic calculation of the mean deviation and mean value for each setting.

> New Work Order

Home

0011 - Testing To

08/01/2018 16:37:16

- Calculates the deviation for each reading, and indicates by colour whether the reading is within tolerance to the selected standard.
- Powerful search function allows historic conformity certificates to be easily found from searching by customer, tool or model; works order number or certificate number.
- Bespoke templates easily created for certificates, reports and labels.
- Auto or manual certificate numbering.
- Tool performance & data input via COM port and keyboard. Option for bar code direct entry.
- Databases can be stored locally or on a server for more efficient backup.
- Data output and report generation collated and filtered from any combination of good and out of tolerance tools.
- All certificate print details recorded. Enables exact reproduction ensuring full traceability.
- A Miscellaneous Tools feature, allowing storage of non torque tool information for use in recording the calibration of Miscellaneous Tools, generating overdue tool reports, and certificate front pages.

		Select>>	Instrument	Descriptio	in .		Combined expanded mea	
	T - 1013 - 50Nm		2206	10Nm IIT1			device uncertainty (Wr	nd %)
			2356	50Nm IIT1				
		<< Deselect	2492 2812	250Nm IIT 500Nm IIT			Selected measuring d measurement error (b	
			2012	1500him II				
		Lab Tempera	ture "C: 20			Lab H	lumidity %: 40	•
tandard Setup:			Readin	ng Settings:				
6789:2017	O 6789-2003	In-House Standard	N	ominal Torque:	50.0	0 N m		
Standard D	escription			Setting 1:	20% **	10.00		
	ICA: Wrench, torsion or flexic			Setting 2:	60%	30.00		
	ICB: Wrench, rigid housing, w							
	ICC: Wrench, rigid housing, a			Setting 3:	100%	50.00		
	ICD: Screwdriver, with scale. ICE: Screwdriver, with electro					alculate		
	CA: Wrench, adjustible, grad				Hec	alculate		
	2CB: Wrench, fixed adjustme		1			O Clockwise		
	2CC: Wrench, adjustable, nor					CIOCKWISE		
	2CD: Screwdriver, adjustible.				0	Counter Clock		
		<u> </u>	(** or los	vest scale grade	uation)			
Comments:		Selection:		c	onformity Sel	ected **	Control	
		Conformity, 6789-20 5 Readings + 3 Exer Tolerance (6%)		T1CD:		<u> </u>	Enter Re	adings
		Clockwise Tool Model ID: Not I		-	-		Cancel R	ading

• Exporting of results data as a csv file for use in other programs.

Advanced Data & Measurement Systems is a Trading name owned by Advanced Witness Systems Ltd © 2024 Data was correct at time of publication. Catalogue Page 59

OTHER FEATURES INCLUDE

- Option to operate in 6789:2003 to allow phased migration to 6789:2017.
- Cloning facility speeds multiple tool data entry.
- Multiple operator accounts for users, maintainers & administrators (with passwords).
- Import and Export reports into text or spreadsheet formats for more efficient database backup.
- Databases can be converted from Kepler 3, 2002 and 2000 allowing faster start up for previous customers.
- Multiple translations available, including the facility to create your own translation.
- Comprehensive user manual.
- Free demonstration and 6 months full help and support included in purchase.
- Certificate conversion available on enquiry.

System Requirements:

Minimum Screen Resolution: 1280x768. Software is a .NET application using an SQL Database. Minimum System: i5 Processor or equivalent, 4GB RAM, on board graphics. Keyboard & Mouse Interface.

Disclaimer: This datasheet may not reflect the latest version of the software. For more information, visit our website: www.awstorque.co.uk.

Also Available: Kepler 4 for Calibra	TION, AND KEPLER 4 COMBINED
•	ystems is a Trading name owned by Systems Ltd © 2024
MANUFACTURER INFORMATION Advanced Witness Systems Ltd Unit 8 Beaumont Business Centre Beaumont Close Banbury OX16 1TN Tel: +44 (0)1295 266939 Email: sales@awstorque.co.uk	SUPPLIER INFORMATION
	it time of publication. le Page 60

eadings: Regular R		Nominal Torque: 50.00	0 N.m Tolerance: 4%	Reading Control:
Setting:	Setting 1 10.000 N.m	Setting 2 Setting 3 30.000 N.m 50.000 N.m	TOMARUA. 476	** Conformity Selected ** Save and Continue
Tolerance: Reading 1:	0.400 N.m 10.000	1.200 N.m 2.000 N.m 30.000 50.000		Clear These Readings Review All Readings
Reading 2: Reading 3:	10.000 9.000	30.000 43.000 30.000 50.000		Restart All Readings
rple=4 Control	New Works Order			Reporting Settings
rrent Works Order: /orks Order Details: Works Order No. 2 CUST1 - Customer 1 TOOL1 - Testing Tool	K000500/03 Check Works Order	Browse Works Orders All Works Orders Unassigned By Selected Customer By Selected Customer[Tool	Selected Customer/Tool: Customer D: CUST1 Customer 1 Vew Customer Lat All Customer Tool D: TOOL1 Testing Tool	Check Custor Edit Customer New Custor Check Too
Readings Complete 18/01/2018 09 02:27 Calibration Reading Calibration	425-31-838-1 SelectCust/Tool	Works Order Action: Update Comment/Tool Add Rending Details View Works Order	View Tool List All Tools	Edit Tool New Tool Customer/Tool Action: View All Readings
				Care Page Defaults



KEPLER 4 FOR CALIBRATION

The program for the calibration of torque wrenches to BS EN ISO 6789:2017 Part 2, BS EN ISO 6789:2003 or your own in-house standards, and for keeping track of each individual wrench.



.....

Save Page Defaults

Kepler 4 is built around a new works orders database, which ties together the customer, tool, model, reading & certificate.

KEY FEATURES INCLUDE

Complies with BS EN ISO 6789:2017 Part 2, allowing the automatic calculation using new formulae of the mean, deviation and combined uncertainty of each set of readings, for each torque tool.

0

- Powerful search function allows historic calibration and conformity certificates to be easily found from searching by customer, tool or model; works order number or certificate number.
- Calibrates both square and hexagonal drive wrenches.
- Full tracking of tools calibration performance and history. Produce a report listing tools that require calibrating.
- The ability to calculate average values of uncertainties Bod, Bint and BI over the last 10 calibrated tools of the same model.
- Bespoke templates easily created for certificates, reports and labels. Auto or manual certificate numbering.
- Auto or manual certificate numbering.
- Tool performance & data input via COM port and keyboard. Option for bar code direct entry.
- All certificate print details recorded. Enables exact reproduction ensuring full traceability.
- Option to operate in 6789:2003 to allow phased migration to 6789:2017.



- The ability to Colour the Calibration, to apply colour indicators to the results to show whether the deviation is within tolerance for the tool type as defined in ISO 6789:2017 Part 1. This can also be displayed on printed reports.
- A Miscellaneous Tools feature, allowing storage of non torque tool information for use in recording the calibration of Miscellaneous Tools, generating overdue tool reports, and certificate front pages.

Advanced Data & Measurement Systems is a Trading name owned by Advanced Witness Systems Ltd © 2024 Data was correct at time of publication. Catalogue Page 61

OTHER FEATURES INCLUDE

- Exporting of results data as a csv file for use in other programs.
- Cloning facility speeds multiple data entry.
- Import and Export reports into text or spreadsheet formats for more efficient database backup.
- Databases can be converted from Kepler 3, 2002 and 2000 allowing faster start up for previous customers.
- Databases can be stored locally or on a server for more efficient backup.
- Multiple translations available, including the facility to create your own translation.
- Data output and report generation collated and filtered from any combination of good and out of tolerance tools.
- Comprehensive user manual.
- Free demonstration and 6 months full help and support included in purchase.
- Certificate conversion available on enquiry.
- **NEW!** K factor verification to UKAS M3003 Appendix's B and C using external spreadsheet module (Sold Separately).

SYSTEM REQUIREMENTS:

Minimum Screen Resolution: 1280x768. Software is a .NET application using an SQL Database. Minimum System: i5 Processor or equivalent, 4GB RAM, on board graphics. Keyboard & Mouse Interface.

Disclaimer: This datasheet may not reflect the latest version of the software. For more information, visit our website: www.awstorgue.co.uk.

ALSO AVAILABLE: KEPLER 4 FOR CONFORMITY, AND KEPLER 4 COMBINED

Advanced Data & Measurement Systems is a Trading name owned by Advanced Witness Systems Ltd © 2024



....

	Works Customer:	Sample1	San	mple Company 1					Q.
Home •	Order Tool:	ToolSamp	pie1 SAM	A1				Reportin	
ading Details	Readings General	Customer	Tool Stand	Jard OtherRead	dings Calculation	15			Control
Date/Timestamp:	Reading		Settin		Setting		Setting		Available Readings:
30/11/2023 15:14:24	Reading	<i>p</i>	Setta	agi	setting	μ.	Setting	,	30/11/2023 15:22:01
Works Order No	Tool Type/C	lass	Setting		Setting		Setting		0711/2023 08:51:19
Screenshots	Type 1A		20% **		60%		100%		19/05/2023 15:29:41
	Clockwis	0	10.00 N/m		30.00 N m		50.00 N m		22/03/2023 12:04:20
Certificate:			Reading	89	Reading	85	Reading	85	21/03/2023 17:06:56
	F	Reading 1:	10.00	0.000%	30.00	0.000%	50.00	0.000%	21/03/2023 17:06:13 21/03/2023 17:06:28
Tool Capacity:		2	10.00	0.000%	30.00	0.000%	50.00	0.000%	2103/2023 17:05:28
50.00 Nm		3	10.00	0.000%	30.00	0.000%	50.00	0.000%	
50.00 Nem		4:	10.00	0.000%	30.00	0.000%	50.00	0.000%	
Standard:		5:	10.00	0.000%	30.00	0.000%	50.00	0.000%	
ISO6789-2017-T1CA									Print Reading
Reading Type:									Pills romany
As Found									Print Label
As Found									
Calibration Reading	2 Mean Va	alue Otbarl:	10,000	_	30.000		50.000		Extract to CSV
6789:2017	Mean of En			0.000%		0.000%		0.000%	
	Uncertainty Exp		0.227%		0.121%		0.105%		
Retest Date:	Uncertainty In		0.477%		0.371%		0.358%		
View Latest Reading	(** or lowest sca						Colour the Calib		

71

Catalogue Page 62

KEPLER 4 K FACTOR VERIFICATION MODULE


The additional module to verify the K Factor of every calibration of torque wrenches and torque screwdrivers to BS EN ISO 6789:2017 Part 2, or your own inhouse standards.



A new feature of Kepler 4: The inclusion of functions to validate the K Factor, required to calculate the expanded uncertainty of a torque tool during calibration (ISO 6789:2017 Part 2), as per the UKAS document M3003 Appendices B and C, using an external spreadsheet module to calculate an adjusted K factor.

KEY FEATURES INCLUDE

- Automatic calculation of the K factor for up to three calibration settings for situations where the resolution contribution is dominant and/or there are unreliable input parameters as per UKAS M3003 Appendix B (Unreliable Inputs) and Appendix C (Dominant Uncertainty Contributions).
- Applicable to ISO 6789:2017 Part 2 or In-House Calibrations.
- Calibration data from Kepler 4 automatically populates the module with a single button press.
- Coverage factor K calculation for probability of 95.45%
- Resolution (r) is assumed by experience and prior knowledge to be the dominant uncertainty.

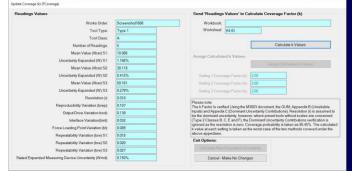

- Where preset tools without scales are concerned (Type 2 Classes B, C, E and F), the Dominant Uncertainty Contributions verification is ignored as the resolution is zero (no scale fitted).
- Removes the difficulty of verifying the K Factor by hand or other spreadsheet means.
- The K Factor Module requires MS Excel to be installed on the computer running Kepler 4.
- K factor verification module sold separately to Kepler 4.

SYSTEM REQUIREMENTS FOR MODULE:

Latest version of Kepler 4 Calibration or Combined Software. Microsoft Excel must be installed on the computer with Kepler 4.

Disclaimer: This datasheet may not reflect the latest version of the software. For more information, visit our website: www.awstorque.co.uk.

ALSO AVAILABLE: KEPLER 4 FOR CONFORMITY, AND KEPLER 4 COMBINED

Advanced Data & Measurement Systems is a Trading name owned by Advanced Witness Systems Ltd © 2024 Data was correct at time of publication. Catalogue Page 63

WIRELESS TELEMETRY LOAD MEASUREMENT

Our Wireless Telemetry Load Measurement System, designed primarily for load lifting systems.

Wireless Telemetry Load Measurement	PAGE
System Overview	65-67
Wireless Telemetry Load Display	68
Wireless Telemetry Load Link	69-70
Wireless Telemetry Load Pin	71-72
Wireless Telemetry Anti 2-Block	73-74

Advanced Witness Systems Ltd Catalogue 2024 Data was correct at time of publication. Catalogue Page 64

DESCRIPTION

The AWS Wireless Telemetry Load Measurement System is designed primarily for load lifting systems.

Multiple Load Links, each with its own digital telemetry transceivers with self-contained batteries, send the data of the loads to a Gateway Router, which acts as a slave Modbus RTU device. In this application a Modbus to Canbus converter to a PLC is part of the full lifting system. The Canbus enables the system to work with the lifting systems Canbus operating data bus. Alternatively, a wireless display may be used over the gateway router for improved portability.

Additional is a Load Pin for an attached jib crane and a safety Anti 2-Block telemetry switch, again self-powered. The Anti 2-Block switch also comes with a weight and chain.

- Each load transducer (link and pin) and Anti 2-Block switch have a unique ident number with which to identify their readings.
- Battery state indicators in the telemetry data show when batteries need changing.
- Each load link and pin is supplied with a calibration certificate traceable to UK national standards.
- The whole system comes programmed ready for use.
- Each cell and unit are to IP67 and operating temperature range of -25 to +55°C.
- Note the router and converter require external power.
- Meets the CE RED directive, and FCC regulations.

For efficient operation, minimum maintenance and long battery life, the load link, load pin and switch go to minimum power requirements until woken up when needed.

This application shown in use in a marina is for lifting large boats/vessels from the water for storage or maintenance with a power driven, hydraulic motors controlled system using a remote portable telemetry, manual operating system. The Load Links tell the operator how much he is lifting and how well balanced. The Load Pin and Anti 2-Block switch enable the operator to lift individual units on and off the vessel.

The systems can also be used in marinas /harbours for jetties, platforms etc., in factories for moving large items such as tanks and engines.



Advanced Witness Systems Ltd © 2024 Data was correct at time of publication. Catalogue Page 65

These are the parts for the system:

TELEMETRY LOAD LINK

- Range 5 to 250 Tonne •
- Transmission Distance up to 200m
- For use with standard shackles
- 5 Step Linearisation
- Auto Power Down
- Sealed to IP67

For more information, please see the Telemetry Load Link Datasheet.

TELEMETRY LOAD PIN

- Strain Gauged Internally
- Capacity 25 Te
- 5 Step Linearisation
- Auto Power Down
- Transmission Distance up to 200m
- Sealed to IP67

For more information, please see the Telemetry Load Pin Datasheet.

TELEMETRY ANTI 2-BLOCK

- Fully weatherproof
- Fail safe operation
- 5 & 10kg bob-weight options
- ATEX version available
- Auto power down
- Transmission distance up to 200m

For more information, please see the Telemetry Anti 2-Block Datasheet.

GATEWAY ROUTER

Email: sales@awstorque.co.uk


- Communicates with all other telemetry modules
- Acts as a Modbus Slave device, storing module readings & status' in read-only registers
- Controls wakeup and sleep of all modules on its network
- Networks can be set up with unique keys, ensuring no clash between nearby operating networks.
- Can be used to control and alarm lifting actuators, engine control generators and pump.

Advanced Witness Systems Ltd © 2024			
MANUFACTURER INFORMATION	SUPPLIER INFORMATION		
Advanced Witness Systems Ltd			
Unit 8			
Beaumont business Centre			
Beaumont Close			
Banbury			
OX16 1TN			
Tel: +44 (0)1295 266939			









CANBUS/MODBUS CONVERTER

- Sends out data held in Modbus registers as Canbus messages
- Canbus message ID matches the telemetry module ID
- Can be used to control and alarm lifting actuators, engine control generators and pumps using the Canbus message system

WIRELESS TELEMETRY LOAD DISPLAY

- Performs advanced operations with telemetry module readings for local monitoring
- Can be configured to perform individual load link/ load cell measurements or in combinations to show such things as bow or stern load when lifting boats or as a total load measurement
- Range of 800m
- For more information, please see the Load Display Datasheet.

EXTERNAL ANTENNA FOR GATEWAY ROUTER

- Replaces the Gateway Router's internal antenna for when the Gateway Router is mounted within a metal enclosure, so that the antenna can be mounted externally.
- 60cm cable attached to Antenna as standard, but additional 3m and 5m extensions are available.
- Range of 800m.









MODEL 6007





Advanced Witness Systems Ltd © 2024 Data was correct at time of publication. Catalogue Page 67



WIRELESS TELEMETRY LOAD DISPLAY

DESCRIPTION

The Wireless Telemetry Load Display allows users to perform advanced operations with load link and load cell readings for local monitoring. It can be configured to perform individual load link/ load cell measurements or in combinations to show such things as bow or stern load when lifting boats or as a total load measurement.




Specifications

- Range of 800m
- Supports two modes of operation -
 - Pre-configured list (Define a set of up to 24 telemetry modules, such as load links, load pins etc. and configure overload and under load values)
 - Summing groups (Add the value of two or more telemetry modules together)
- Sealed to IP67 in a robust handheld enclosure
- ATEX version available

Features & Benefits

- Simple operator interface
- Overload indication and alarm
- User controlled backlight
- Tare/ Zero/ Gross functions
- Uses readily available Energizer L91 batteries
- Long battery life: 50 days at 12 sessions of 5 minutes per day; 54 hours continuous
- Operating temperature range of -10°C to +50°C

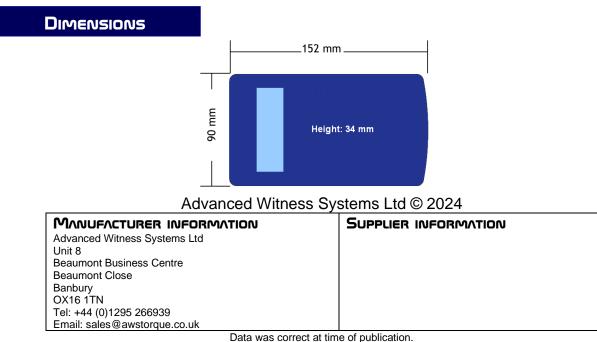

WIRELESS TELEMETRY LOAD LINK

DESCRIPTION

The Wireless Telemetry Load Link is a strain gauged link with an inbuilt battery powered wireless transceiver which communicates with our AWS Wireless Telemetry Load Measurement System. With a simple to change extra-long life battery, and a large range of load capacities, it is ideal for applications in systems where running cables to a load link is not possible.



SPECIFICATIONS

- Range 5 to 250 Tonne
- Transmission Distance up to 200m
- For use with standard shackles
- 5 Step Linearisation
- Auto Power Down
- Sealed to IP67
- Meets the CE RED directive, and FCC regulations.

FEATURES & BENEFITS

- Long battery life
- Error free data transmission
- Active repeater to extend transmission range
- Remote on/off
- Environmentally sealed
- Internal aerial
- Other capacities available on request


Specifications		
Capacities	5-250	tonne
Radio Frequency	2.4	GHz
Accuracy (above 10% of FSD)	±0.05	% of reading
Compensated Temp. Range	-10 to +40	°C
Operating Temp. Range	-20 to +60	°C
Temp. Coefficient on Zero	<0.005	% FRO/°C
Temp. Coefficient on Span	< 0.003	% FRO/°C
Safe Overload	150	%
Ultimate Overload	400	%
Insulation	>500 @100Vdc	MΩ
Environmental Protection	IP67	

Specifications subject to change without notice

DIMENSIONS

Capacity (te)	A	В	С	DØ	E	Weight (Kg)
5	137	105	41.5	30	193	1.5
12	149	105	41.5	38	239	2.0
25	160	125	55	53	284	4.5
35	175	138	55	60	335	5.5
50	198	150	75	73	375	10.0
100	275	220	120	100	500	28.0
150	300	260	120	110	550	50.0
200	325	290	159	135	660	75.0
250	365	304	189	145	720	90.0

All dimensions in mm

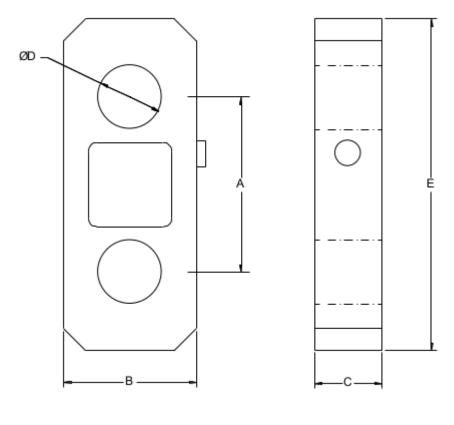

Advanced Witness Systems Ltd © 2024

MANUFACTURER INFORMATION Advanced Witness Systems Ltd Unit 8

Beaumont business Centre Beaumont Close Banbury Ox16 1TN Tel: +44 (0)1295 266939 Email: sales@awstorque.co.uk

SUPPLIER INFORMATION

Data was correct at time of publication. Catalogue Page 70

WIRELESS TELEMETRY LOAD PIN

DESCRIPTION

The Wireless Telemetry Load Pin is a strain gauged pin with a local battery powered wireless transceiver which communicates with our AWS Wireless Telemetry Load Measurement System. With a simple to change extra-long life battery, and a large range of load capacities, it is ideal for applications in systems where running cables to a load pin is not possible. The transceiver can be mounted within 3m of the Load Pin, in an easy to access location for battery changing.



Specifications


- Stainless Steel
- Strain Gauged Internally
- Capacity 25 Te
- 5 Step Linearisation
- 3m cable from Load Pin to its transceiver
- Auto Power Down
- Transmission Distance up to 200m
- Sealed to IP67
- Meets the CE RED directive, & FCC regulations.

FEATURES & BENEFITS

- Long battery life
- Error free data transmission
- Active repeater to extend transmission range
- Remote on/off
- Environmentally sealed
- Other capacities available on request

Specification		
Capacity	5-1000	tonne
Radio Frequency	2.4	GHz
Accuracy (above 10% of FSD)	±0.05	% of reading
Compensated Temp. Range	-10 to +40	°C
Operating Temp. Range	-20 to +60	°C
Temp. Coefficient on Zero	<0.005	% FRO/°C
Temp Coefficient on Span	<0.003	% FRO/°C
Safe Overload	150	%

DIMENSIONS

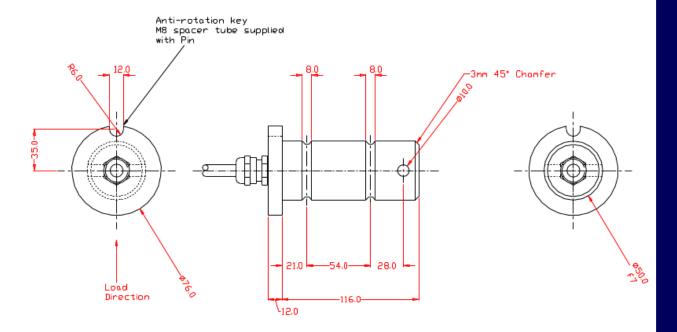

Advanced Witness Systems Ltd © 2

MANUFACTURER INFORMATION	SUPPLIER INFORMATION
Advanced Witness Systems Ltd	
Unit 8	
Beaumont Business Centre	
Beaumont Close	
Banbury	
OX16 1TN	
Tel: +44 (0)1295 266939	
Email: sales@awstorque.co.uk	

WIRELESS TELEMETRY ANTI 2-BLOCK

DESCRIPTION

The Wireless Telemetry Anti 2-Block is an Anti 2-Block detector with a local battery powered wireless transceiver which communicates with our AWS Wireless Telemetry Load Measurement System. It is ideal for applications in systems where running cables to an Anti 2-Block is not possible. The transceiver can be mounted within 3m of the Anti 2-Block, in an easy to access location for battery changing. It can be supplied with or without its weight & chain.




SPECIFICATIONS

- Robust construction for reliability
- Fully weatherproof
- Fail safe operation
- 5 & 10kg bob-weight options
- 3m cable from Anti 2-Block to its transceiver
- ATEX version available
- Simple to install
- Auto power down
- Transmission distance up to 200m
- Meets the CE RED directive, and FCC regulations.

FEATURES & BENEFITS

- Long battery life
- Error free data transmission
- Active repeater to extend transmission range
- Remote on/off
- Environmentally sealed
- Contacts are broken mechanically
- Unit pivots from boom head & always follows the angle of the hoist rope



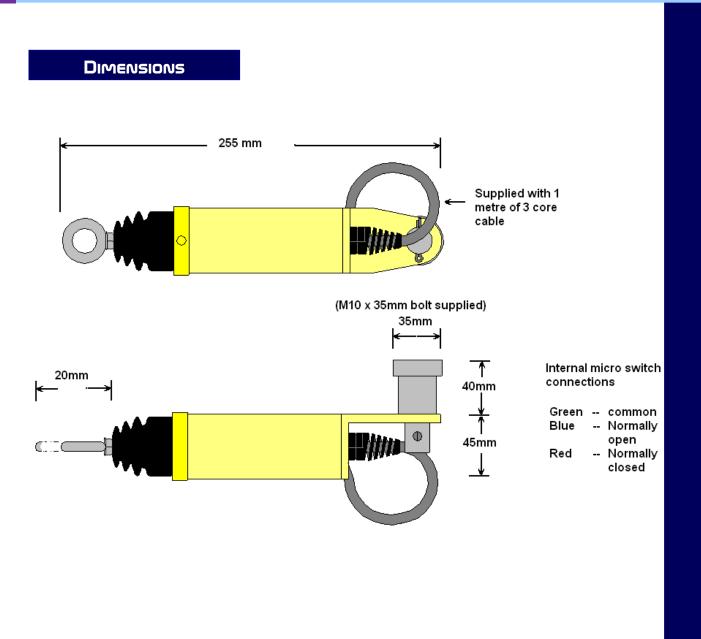

Advanced Witness Systems Ltd © 2024

MANUFACTURER INFORMATION	SUPPLIER INFORMATION
Advanced Witness Systems Ltd	
Unit 8	
Beaumont Business Centre	
Beaumont Close	
Banbury	
OX16 1TN	
Tel: +44 (0)1295 266939	
Email: sales@awstorque.co.uk	



Advanced Witness Systems Ltd Unit 8, Beaumont Business Centre, Beaumont Close

Unit 8, Beaumont Business Centre, Beaumont Close Banbury, Oxfordshire OX16 1TN Telephone: +44(0)1295 266939 sales@awstorque.co.uk www.awstorque.co.uk